

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025465.D
 Acq On : 12 Apr 2022 10:22
 Operator : SY/MD
 Sample : VV0412WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK340

Quant Time: Apr 13 02:31:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	132050	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	132492	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	62151	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	49086	3.998	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.568	69	48350	3.702	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	74.000%
11) 1,1-Dichloroethene-d2	2.105	63	79178	3.219	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.400%
20) 2-Butanone-d5	3.899	46	69634	46.629	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.260%
24) Chloroform-d	4.343	84	79747	4.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.031	65	37266	4.662	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.047	84	156835	4.091	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
36) 1,2-Dichloropropane-d6	6.063	67	46352	4.336	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.800%
41) Toluene-d8	7.314	98	131795	3.705	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.000%
43) trans-1,3-Dichloroprop...	7.622	79	13167	3.664	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.200%
46) 2-Hexanone-d5	8.088	63	50760	40.248	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.500%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29285	4.336	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	47126	4.523	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.400%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	2583	0.233	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025465.D
Acq On : 12 Apr 2022 10:22
Operator : SY/MD
Sample : VV0412WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK340


Quant Time: Apr 13 02:31:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 13 02:31:13 2022
Response via : Initial Calibration

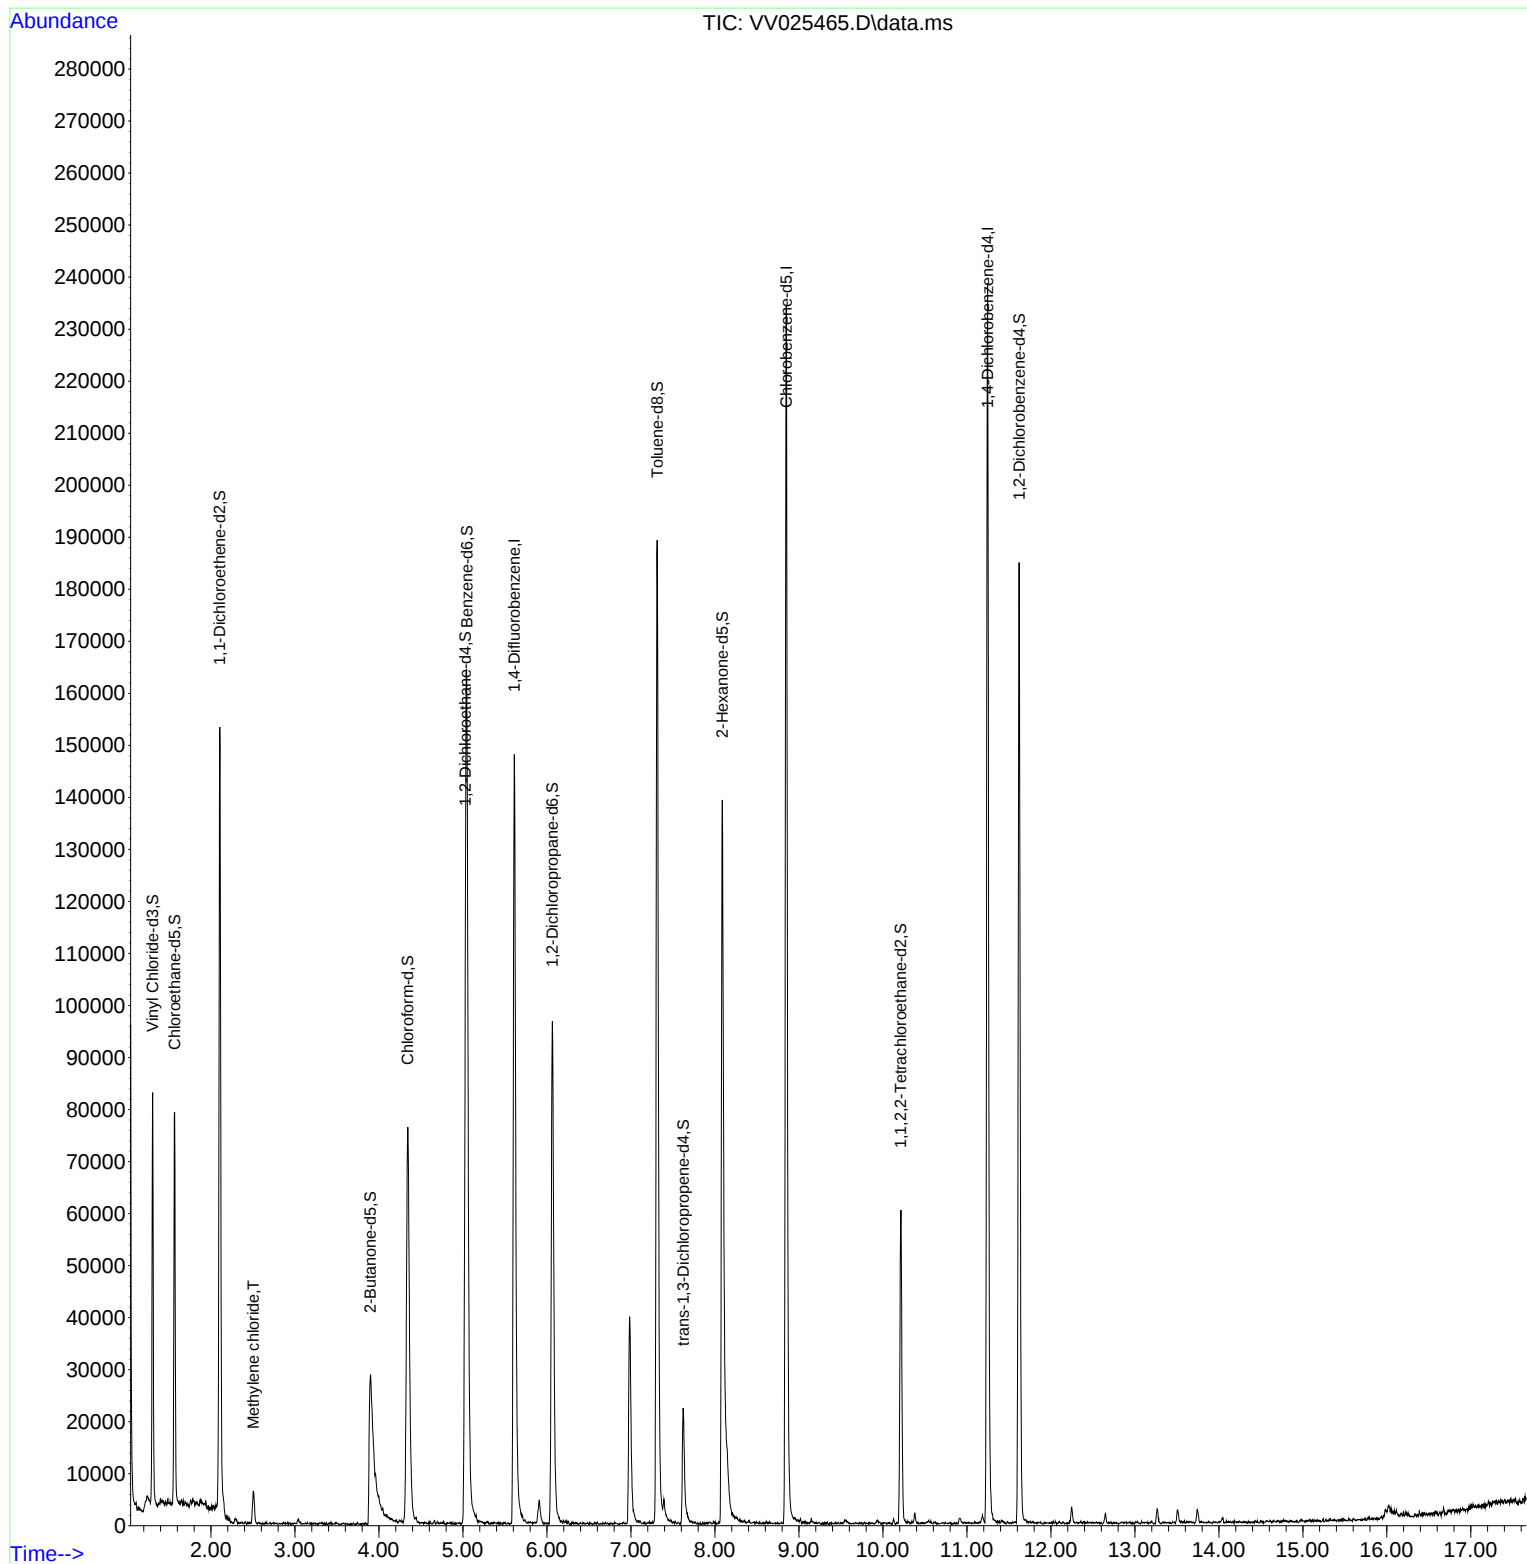

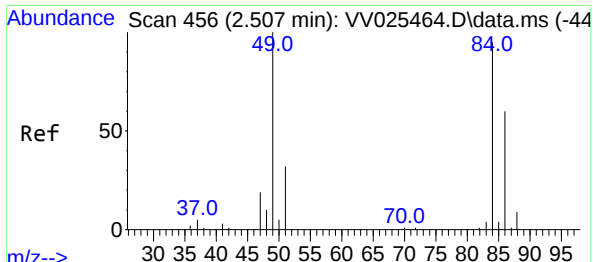

#16
Methylene chloride
Concen: 0.233 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV025465.D
Acq: 12 Apr 2022 10:22

Instrument :
MSVOA_V
ClientSampleId :
VBLK340

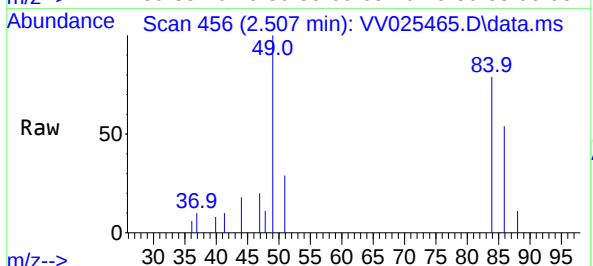

Tgt Ion: 84 Resp: 2583

Ion	Ratio	Lower	Upper
84	100		
86	69.2	45.9	85.3
49	127.2	76.6	142.3

