

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041222\
 Data File : VW025466.D
 Acq On : 12 Apr 2022 11:01
 Operator : SY/MD
 Sample : N2289-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 13 02:31:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	135823	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	137061	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	64581	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	48812	3.865	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.400%
7) Chloroethane-d5	1.568	69	48005	3.573	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.400%
11) 1,1-Dichloroethene-d2	2.108	63	79818	3.155	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.200%
20) 2-Butanone-d5	3.895	46	74818	48.709	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.420%
24) Chloroform-d	4.346	84	81949	4.295	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
26) 1,2-Dichloroethane-d4	5.030	65	38900	4.731	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
32) Benzene-d6	5.047	84	158915	4.007	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.200%
36) 1,2-Dichloropropane-d6	6.066	67	47486	4.294	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.800%
41) Toluene-d8	7.313	98	133059	3.616	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.400%
43) trans-1,3-Dichloroprop...	7.622	79	14646	3.940	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.800%
46) 2-Hexanone-d5	8.085	63	52840	40.500	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.000%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30130	4.312	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	47919	4.426	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.600%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	3907	0.342	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025466.D
Acq On : 12 Apr 2022 11:01
Operator : SY/MD
Sample : N2289-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Apr 13 02:31:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 13 02:31:13 2022
Response via : Initial Calibration

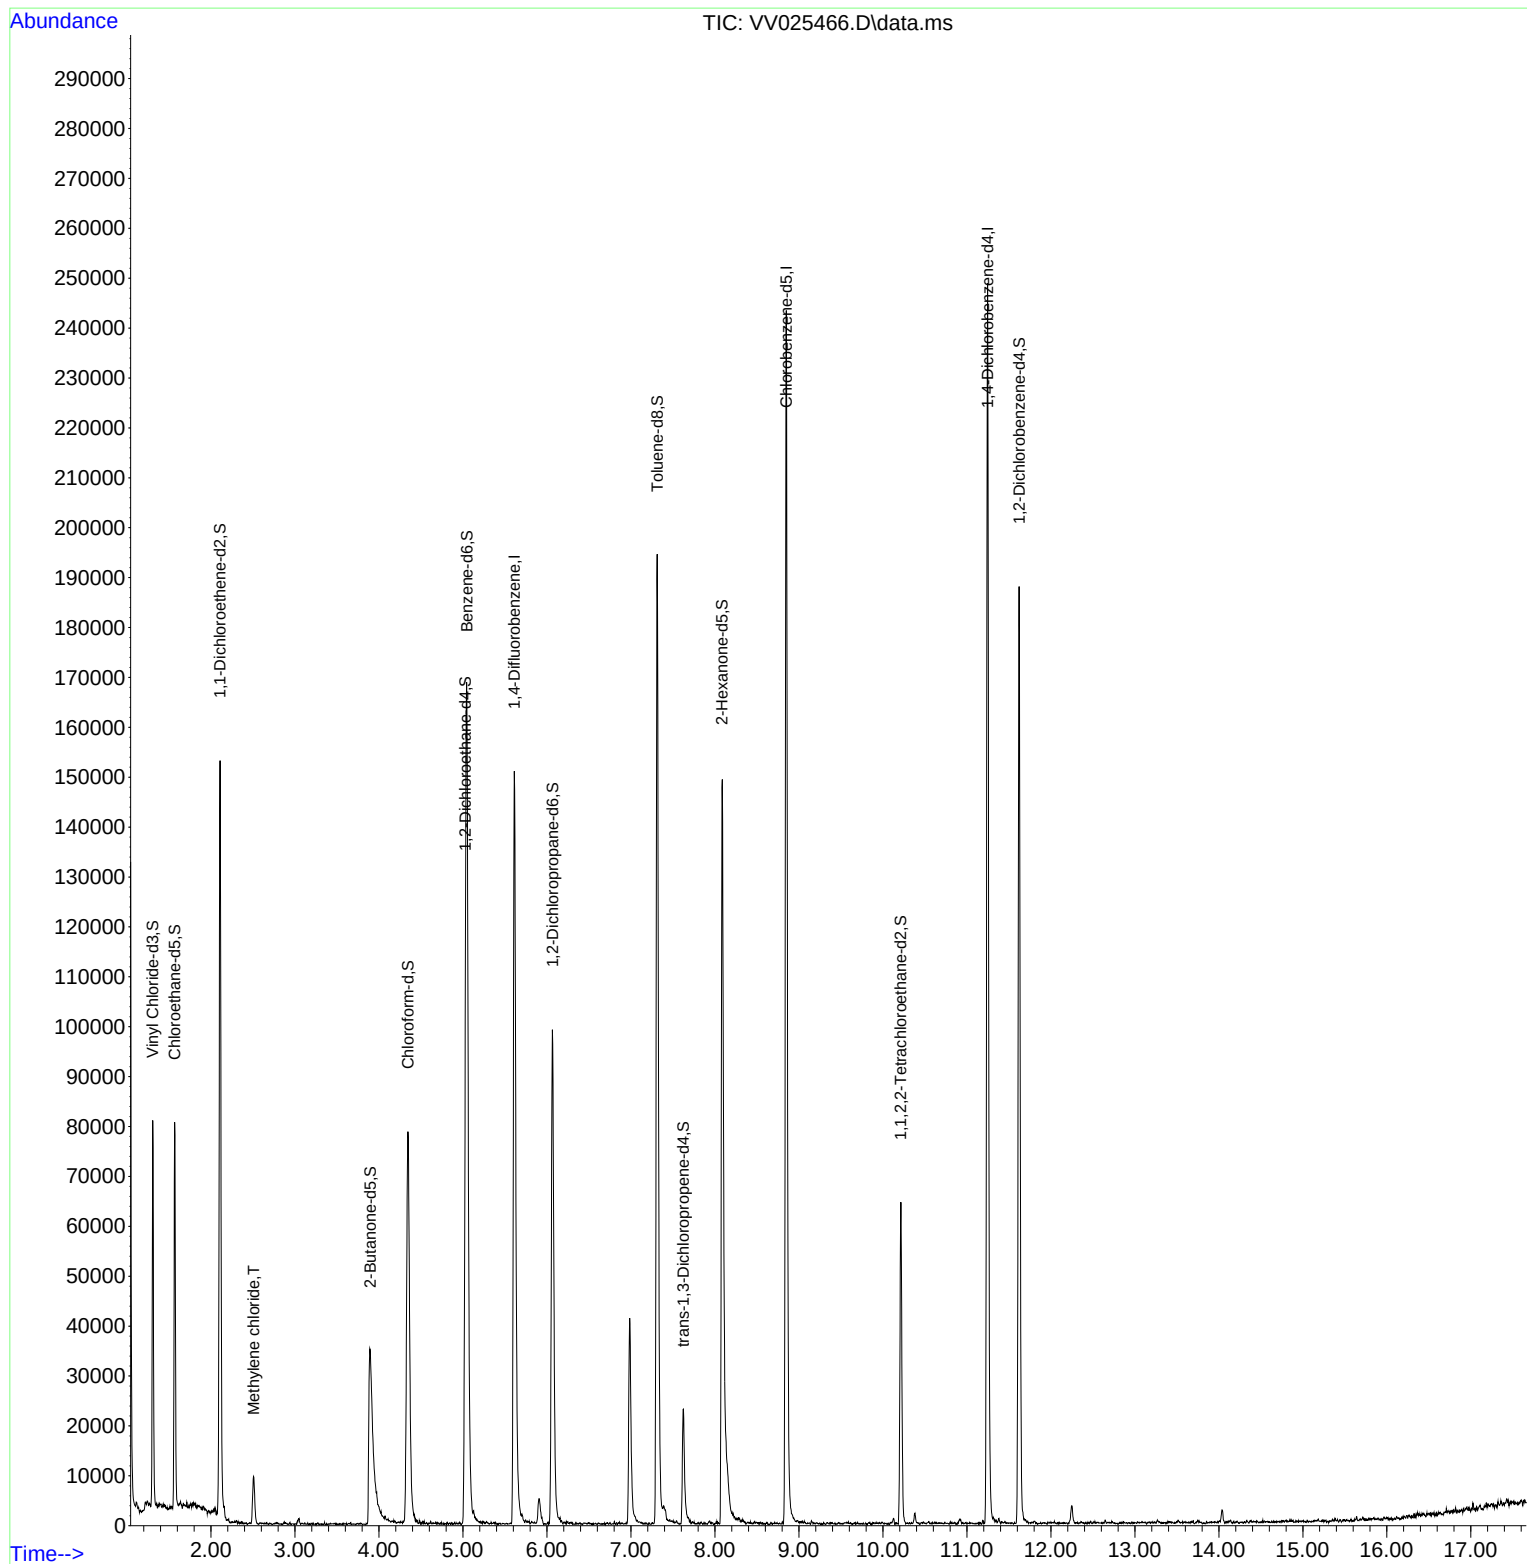

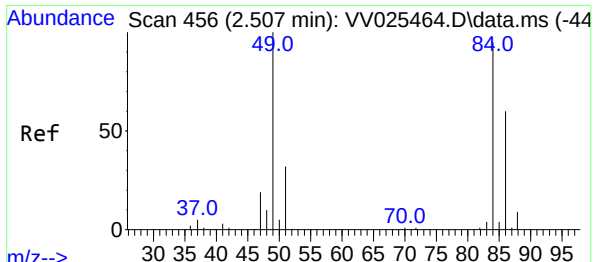

#16
Methylene chloride
Concen: 0.342 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025466.D
Acq: 12 Apr 2022 11:01

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

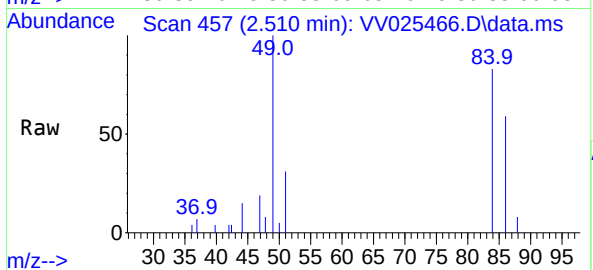

Tgt Ion: 84 Resp: 3907
Ion Ratio Lower Upper
84 100
86 71.2 45.9 85.3
49 120.3 76.6 142.3

