

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041222\
 Data File : VW025467.D
 Acq On : 12 Apr 2022 11:24
 Operator : SY/MD
 Sample : N2357-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAZ02

Quant Time: Apr 13 02:32:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	126668	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	129214	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58730	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56049	4.759	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.200%
7) Chloroethane-d5	1.568	69	52335	4.177	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.600%
11) 1,1-Dichloroethene-d2	2.108	63	88321	3.744	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.800%
20) 2-Butanone-d5	3.905	46	65328	45.605	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.200%
24) Chloroform-d	4.352	84	83570	4.696	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
26) 1,2-Dichloroethane-d4	5.037	65	39801	5.191	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.050	84	164559	4.402	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
36) 1,2-Dichloropropane-d6	6.069	67	48879	4.688	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.800%
41) Toluene-d8	7.316	98	138237	3.984	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	7.625	79	12647	3.609	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.200%
46) 2-Hexanone-d5	8.091	63	52673	42.824	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.640%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31931	4.847	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	47882	4.863	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.200%
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.297	76	5077	0.193	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025467.D
Acq On : 12 Apr 2022 11:24
Operator : SY/MD
Sample : N2357-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ02


Quant Time: Apr 13 02:32:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 13 02:31:13 2022
Response via : Initial Calibration

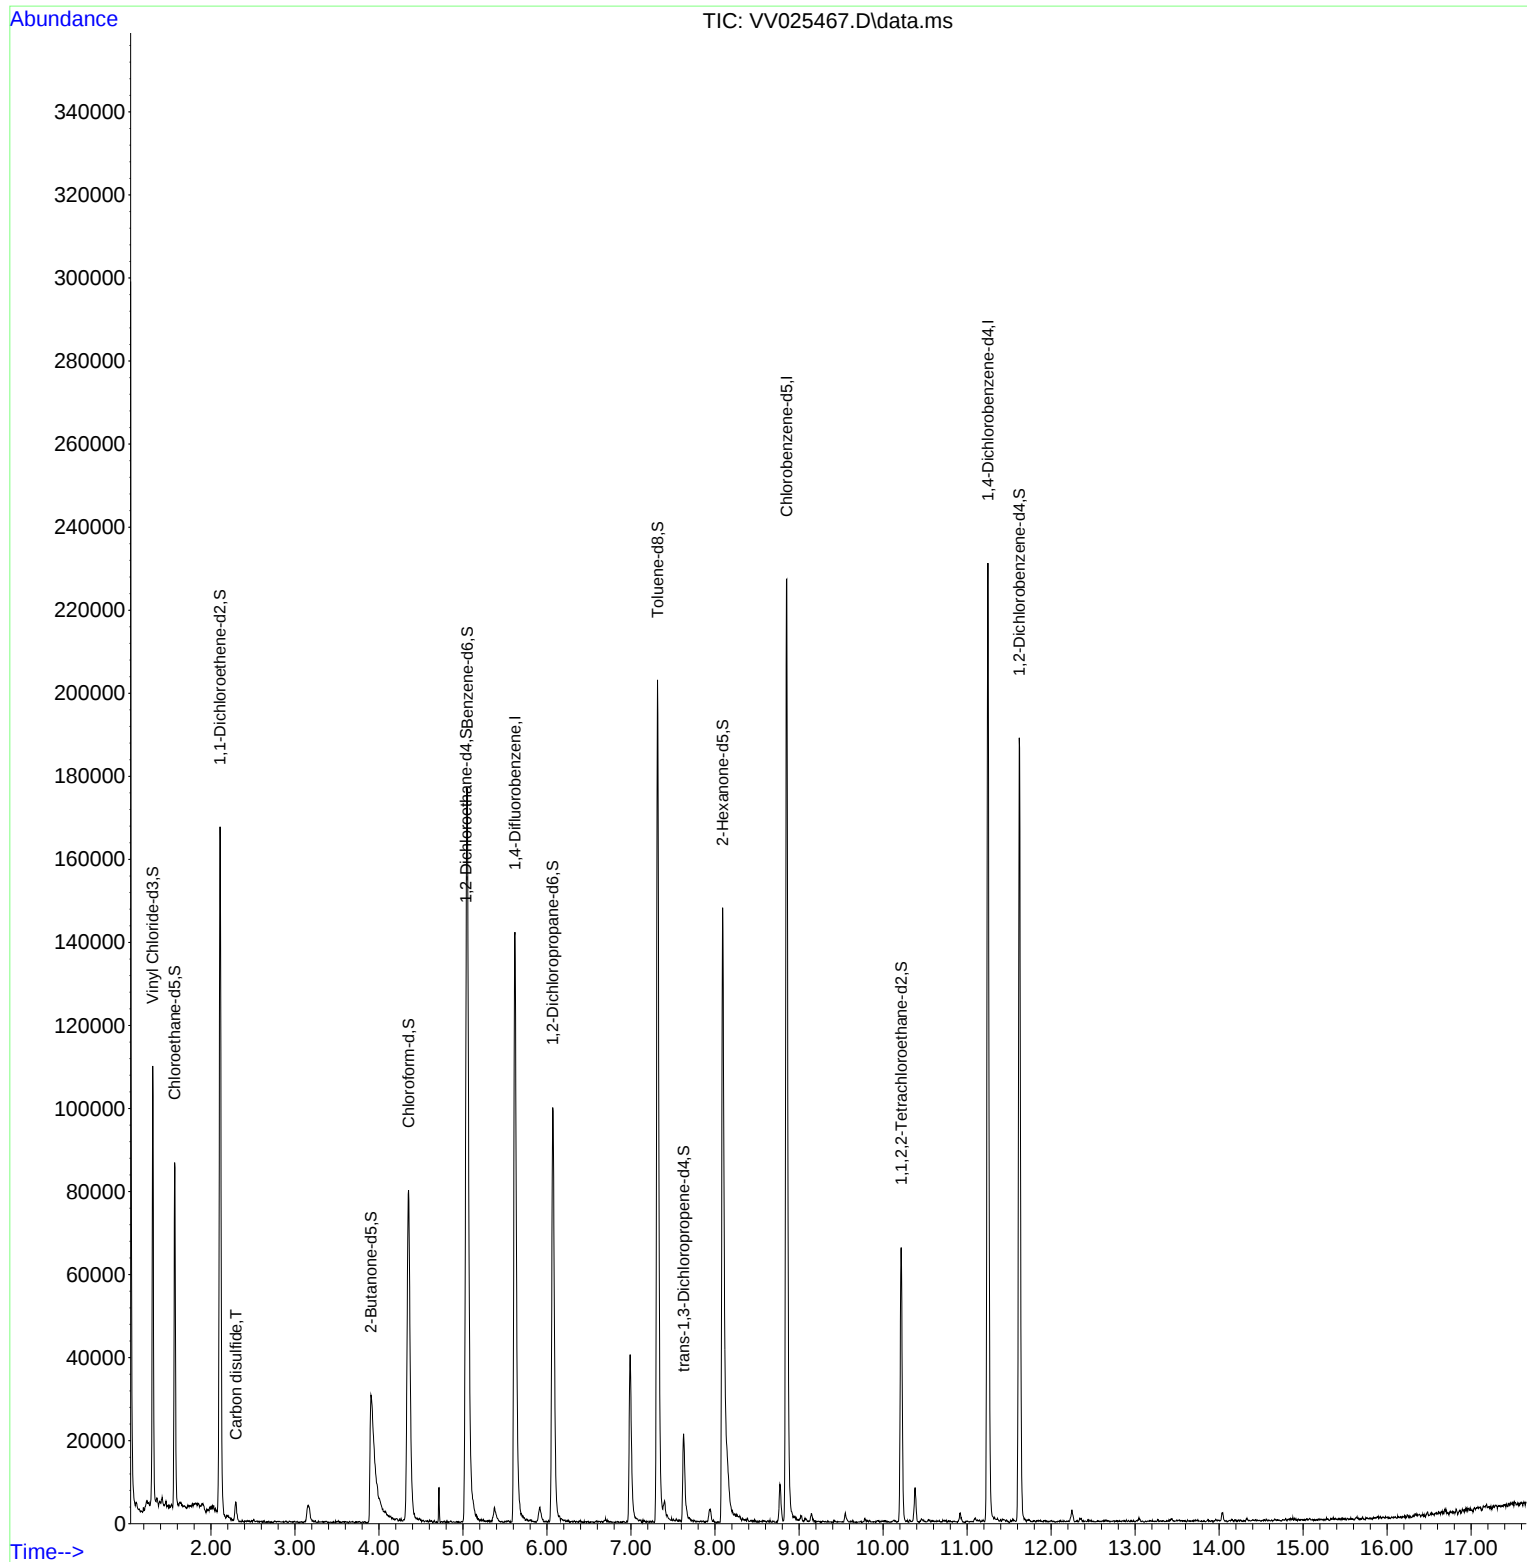

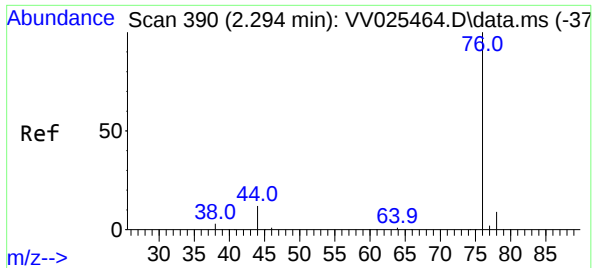

#14
Carbon disulfide
Concen: 0.193 ug/L
RT: 2.297 min Scan# 391
Delta R.T. 0.003 min
Lab File: VV025467.D
Acq: 12 Apr 2022 11:24

Instrument :
MSVOA_V
ClientSampleId :
YAZ02

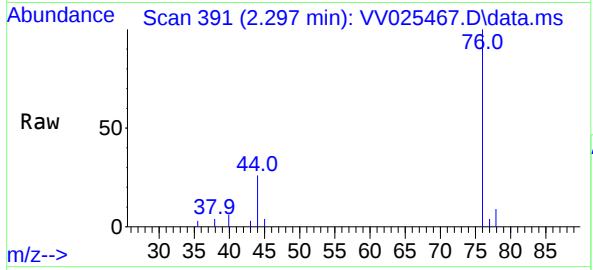

Tgt Ion: 76 Resp: 5077
Ion Ratio Lower Upper
76 100
78 9.5 7.3 10.9

