

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041222\
 Data File : VW025471.D
 Acq On : 12 Apr 2022 13:57
 Operator : SY/MD
 Sample : N2356-25
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDW5

Quant Time: Apr 13 02:33:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	137381	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	138861	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	76093	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	45349	3.551	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.000%
7) Chloroethane-d5	1.571	69	44187	3.252	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	65.000%
11) 1,1-Dichloroethene-d2	2.111	63	119458	4.669	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.400%
20) 2-Butanone-d5	3.896	46	73871	47.547	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.100%
24) Chloroform-d	4.349	84	81356	4.215	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
26) 1,2-Dichloroethane-d4	5.031	65	36455	4.384	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
32) Benzene-d6	5.047	84	150891	3.756	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.200%
36) 1,2-Dichloropropane-d6	6.069	67	45331	4.046	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.000%
41) Toluene-d8	7.313	98	126733	3.399	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.000%#
43) trans-1,3-Dichloroprop...	7.622	79	13457	3.573	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.400%
46) 2-Hexanone-d5	8.088	63	52726	39.889	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.780%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30524	4.312	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	47291	3.707	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	74.200%#
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.130	85	28329	2.283	ug/L	99
3) Chloromethane	1.243	50	108243	8.027	ug/L	96
5) Vinyl chloride	1.314	62	85957	5.641	ug/L	98
6) Bromomethane	1.523	94	45953	4.182	ug/L	100
8) Chloroethane	1.587	64	55305	4.702	ug/L	99
9) Trichlorofluoromethane	1.754	101	247085	11.544	ug/L	99
10) 1,1,2-Trichloro-1,2,2-...	2.117	101	65421	5.441	ug/L	98
12) 1,1-Dichloroethene	2.121	96	83968	7.047	ug/L #	71
16) Methylene chloride	2.507	84	40585	3.513	ug/L	98
17) Methyl tert-butyl Ether	2.770	73	103659	5.622	ug/L	99
18) trans-1,2-Dichloroethene	2.761	96	73962	7.407	ug/L	98
22) cis-1,2-Dichloroethene	3.908	96	73890	7.029	ug/L	94
23) Bromochloromethane	4.256	128	10008	2.293	ug/L #	91
25) Chloroform	4.375	83	97106	5.440	ug/L	98
27) 1,2-Dichloroethane	5.130	62	55312	5.873	ug/L	99
29) 1,1,1-Trichloroethane	4.606	97	95324	5.820	ug/L	98
31) Carbon tetrachloride	4.825	117	83131	6.002	ug/L	99
34) Trichloroethene	5.912	95	99722	9.156	ug/L	99
37) 1,2-Dichloropropane	6.172	63	51996	5.479	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025471.D
 Acq On : 12 Apr 2022 13:57
 Operator : SY/MD
 Sample : N2356-25
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDW5


Quant Time: Apr 13 02:33:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Apr 13 02:31:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


38) Bromodichloromethane	6.510	83	27932	2.371	ug/L	98
39) cis-1,3-Dichloropropene	7.027	75	22633	1.820	ug/L	98
42) Toluene	7.387	91	145511	3.261	ug/L	98
45) 1,1,2-Trichloroethane	7.837	97	57391	9.031	ug/L	100
47) Tetrachloroethene	7.973	164	48761	5.719	ug/L	97
49) Dibromochloromethane	8.243	129	45477	6.519	ug/L	96
52) Ethylbenzene	9.011	91	546279	11.479	ug/L	99
54) o-Xylene	9.542	106	55514	3.159	ug/L	96
55) Styrene	9.561	104	82746	2.896	ug/L	100
57) 1,1,2,2-Tetrachloroethane	10.239	83	33022	5.201	ug/L	99
60) Isopropylbenzene	9.931	105	381043	8.090	ug/L	100
63) 1,2,4-Trimethylbenzene	10.911	105	185989	4.915	ug/L	98
64) 1,3-Dichlorobenzene	11.178	146	49511	2.252	ug/L	98
67) 1,2-Dichlorobenzene	11.641	146	43242	2.221	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 13 02:33:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Apr 13 02:31:13 2022
Response via : Initial Calibration







Abundance Scan 28 (1.130 min): VV025464.D\data.ms (-20)

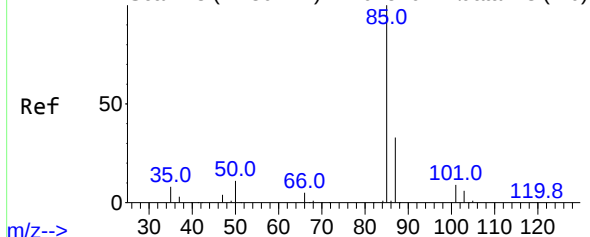

#2
Dichlorodifluoromethane
Concen: 2.283 ug/L
RT: 1.130 min Scan# 28
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion: 85 Resp: 28329
Ion Ratio Lower Upper
85 100
87 32.6 25.6 38.4

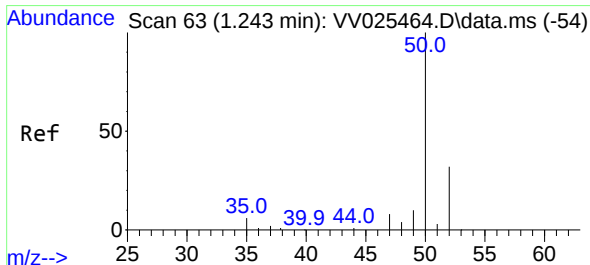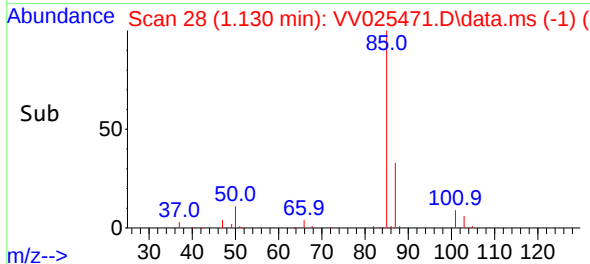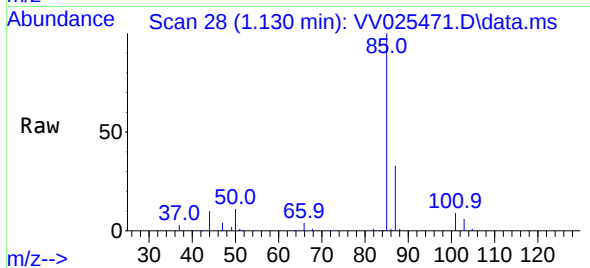

#3
Chloromethane
Concen: 8.027 ug/L
RT: 1.243 min Scan# 63
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 50 Resp: 108243
Ion Ratio Lower Upper
50 100
52 31.7 23.7 43.9


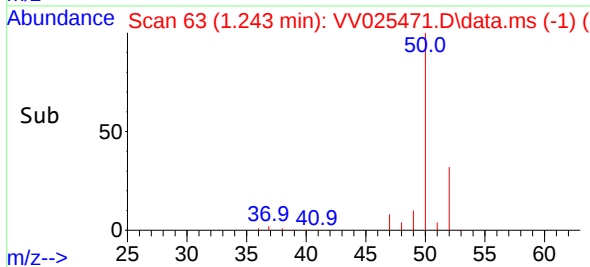

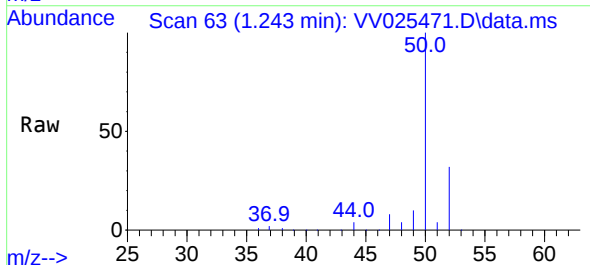


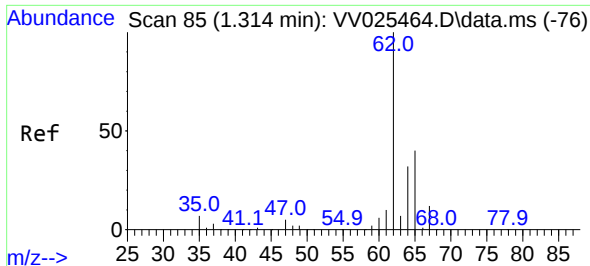

#5
 Vinyl chloride
 Concen: 5.641 ug/L
 RT: 1.314 min Scan# 85
 Delta R.T. 0.000 min
 Lab File: VV025471.D
 Acq: 12 Apr 2022 13:57




Instrument :
 MSVOA_V
 ClientSampleId :
 GBDW5


Tgt Ion: 62 Resp: 85957
 Ion Ratio Lower Upper
 62 100
 64 32.0 23.2 43.2

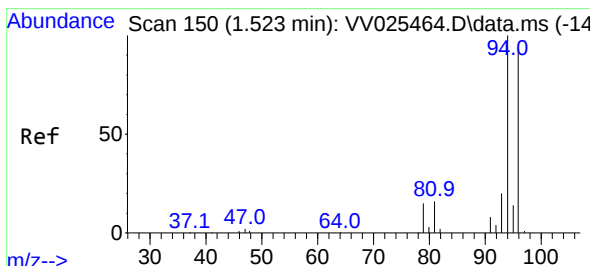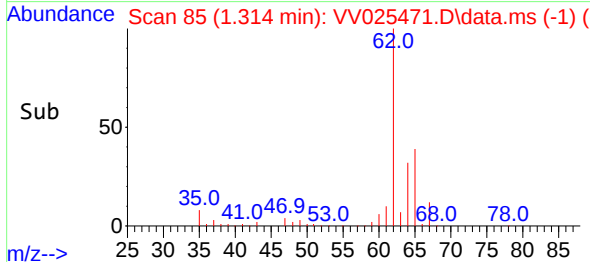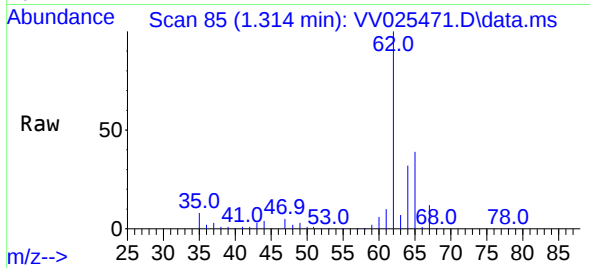

#6
 Bromomethane
 Concen: 4.182 ug/L
 RT: 1.523 min Scan# 150
 Delta R.T. 0.000 min
 Lab File: VV025471.D
 Acq: 12 Apr 2022 13:57

Tgt Ion: 94 Resp: 45953
 Ion Ratio Lower Upper
 94 100
 96 94.2 66.1 122.7


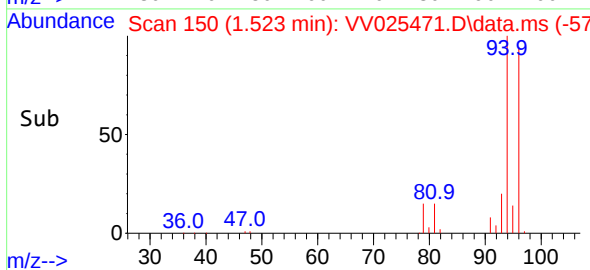

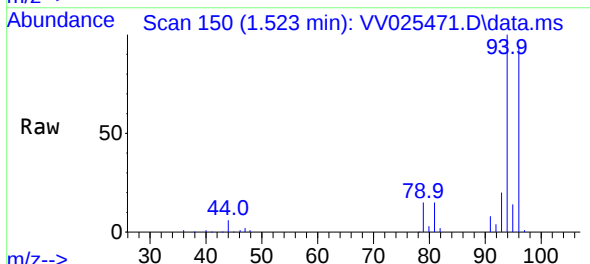




#8
Chloroethane
Concen: 4.702 ug/L
RT: 1.587 min Scan# 11
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion: 64 Resp: 55305
Ion Ratio Lower Upper
64 100
66 30.9 21.8 40.6

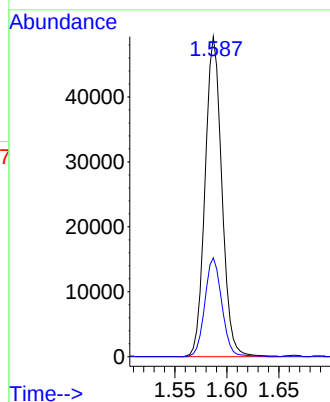

#9
Trichlorofluoromethane
Concen: 11.544 ug/L
RT: 1.754 min Scan# 222
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 101 Resp: 247085
Ion Ratio Lower Upper
101 100
103 64.4 51.9 77.9


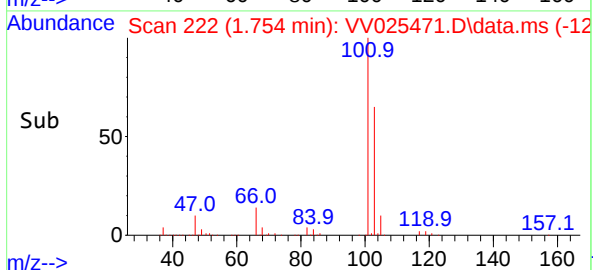




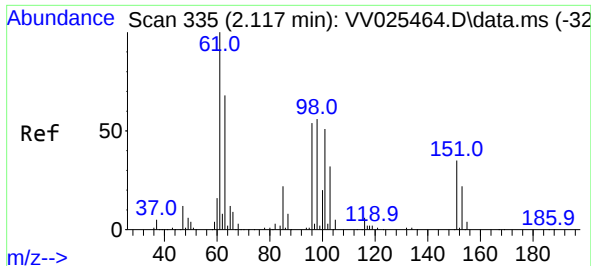

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 5.441 ug/L
RT: 2.117 min Scan# 31
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion:101 Resp: 65421
Ion Ratio Lower Upper
101 100
85 45.6 35.9 53.9
151 68.0 56.0 84.0

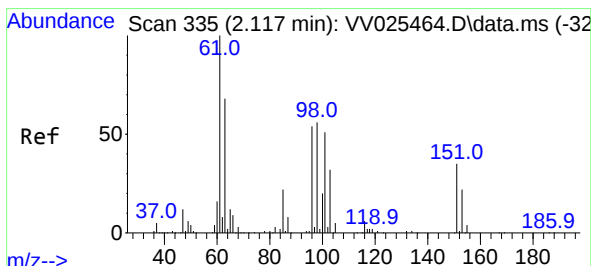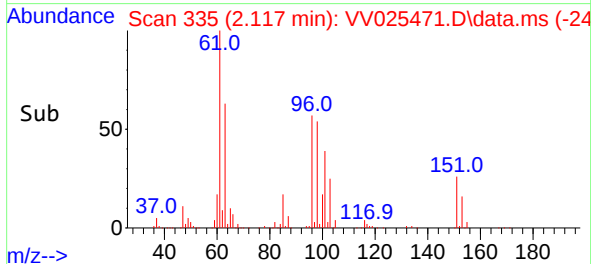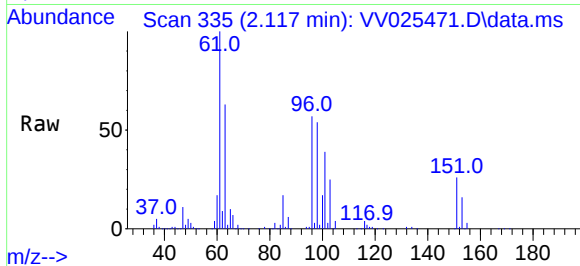

#12
1,1-Dichloroethene
Concen: 7.047 ug/L
RT: 2.121 min Scan# 336
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 96 Resp: 83968
Ion Ratio Lower Upper
96 100
61 170.6 125.2 232.4
63 91.1 114.4 212.4#


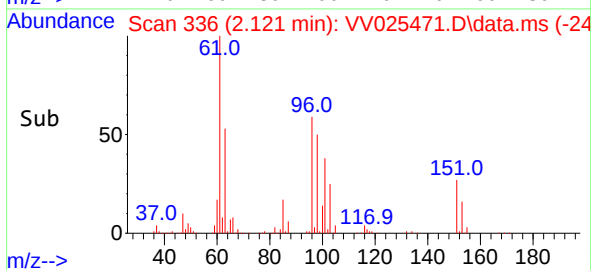

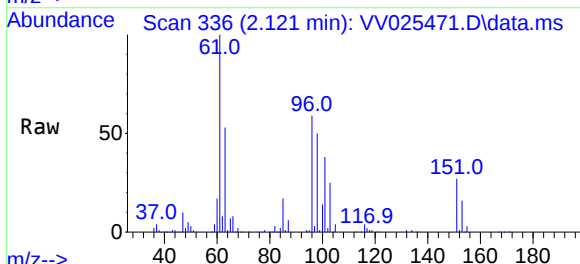




#16
Methylene chloride
Concen: 3.513 ug/L
RT: 2.507 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion:	84	Resp:	40585
Ion	Ratio	Lower	Upper
84	100		
86	62.8	45.9	85.3
49	109.9	76.6	142.3



#17
Methyl tert-butyl Ether
Concen: 5.622 ug/L
RT: 2.770 min Scan# 538
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion:	73	Resp:	103659
Ion	Ratio	Lower	Upper
73	100		
43	17.4	14.2	21.4
57	20.7	16.1	24.1


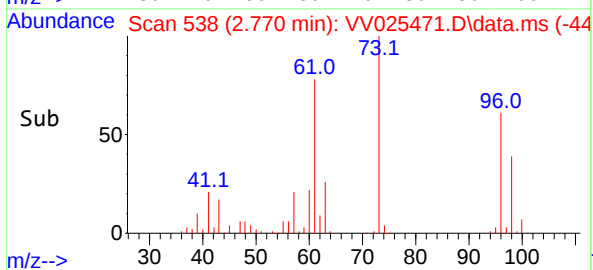




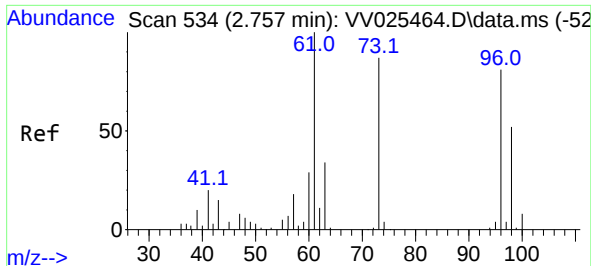

#18
trans-1,2-Dichloroethene
Concen: 7.407 ug/L
RT: 2.761 min Scan# 51
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion: 96 Resp: 73962
Ion Ratio Lower Upper
96 100
61 130.4 92.1 171.1
98 63.9 47.5 88.1

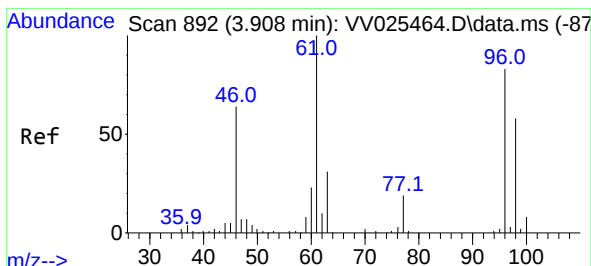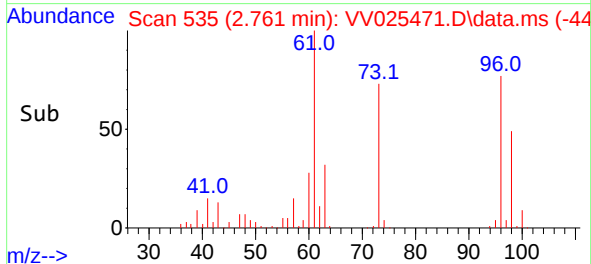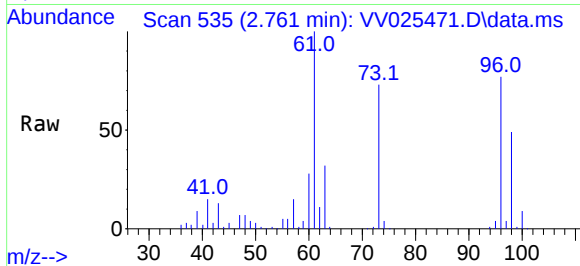

#22
cis-1,2-Dichloroethene
Concen: 7.029 ug/L
RT: 3.908 min Scan# 892
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57


Tgt Ion: 96 Resp: 73890
Ion Ratio Lower Upper
96 100
61 120.6 80.0 148.6
68 0.0 0.0 0.0

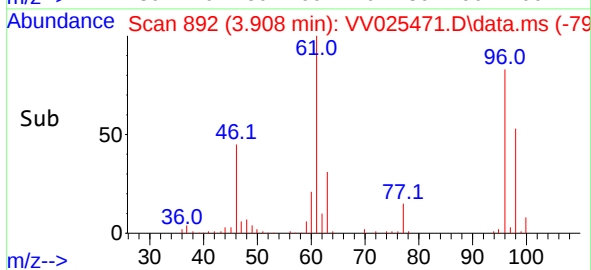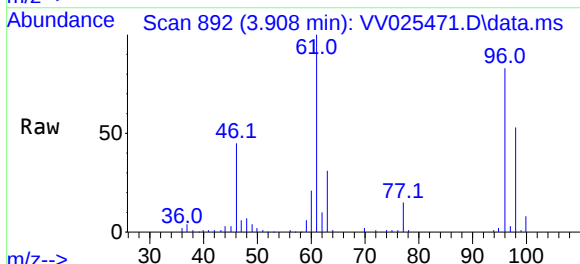






#23
Bromochloromethane
Concen: 2.293 ug/L
RT: 4.256 min Scan# 1000
Delta R.T. 0.010 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Instrument :
MSVOA_V
ClientSampleId :
GBDW5



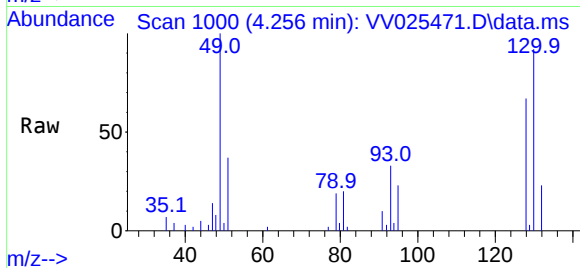



Tgt Ion:128 Resp: 10008
Ion Ratio Lower Upper
128 100
49 149.5 100.5 186.7
130 138.1 87.8 163.0
51 56.0 35.1 52.7#

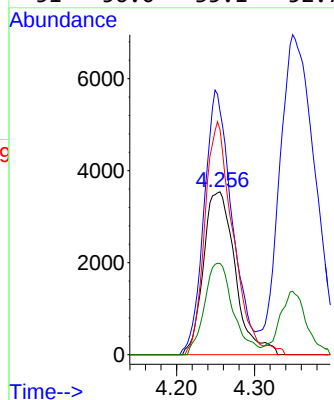

#25
Chloroform
Concen: 5.440 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 83 Resp: 97106
Ion Ratio Lower Upper
83 100
85 63.7 43.5 80.7


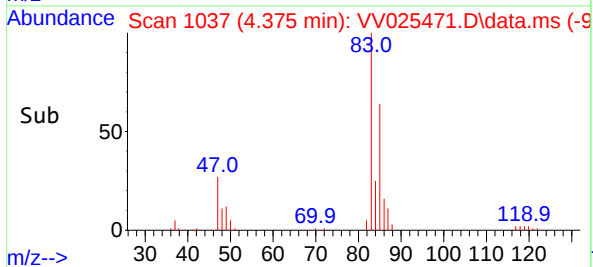
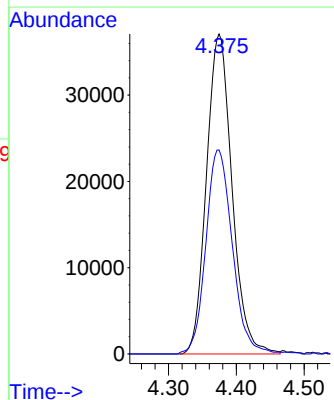
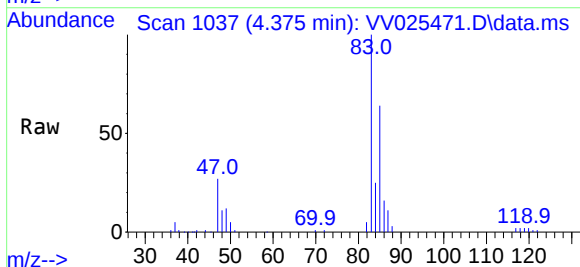




#27
1,2-Dichloroethane
Concen: 5.873 ug/L
RT: 5.130 min Scan# 1109
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion: 62 Resp: 55312
Ion Ratio Lower Upper
62 100
98 10.5 8.8 13.2

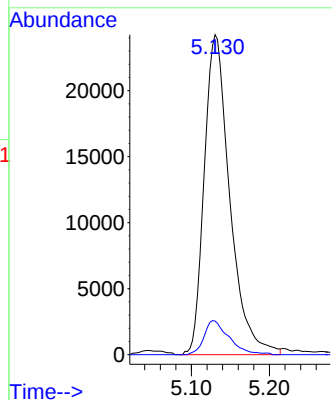

#29
1,1,1-Trichloroethane
Concen: 5.820 ug/L
RT: 4.606 min Scan# 1109
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 97 Resp: 95324
Ion Ratio Lower Upper
97 100
99 62.0 51.5 77.3
61 42.7 34.3 51.5


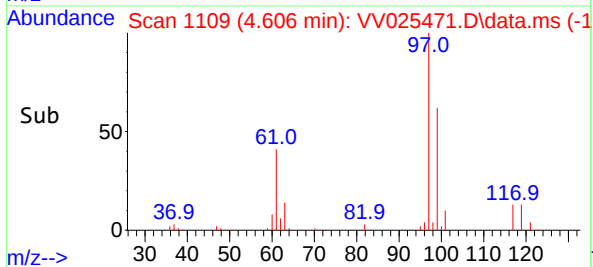
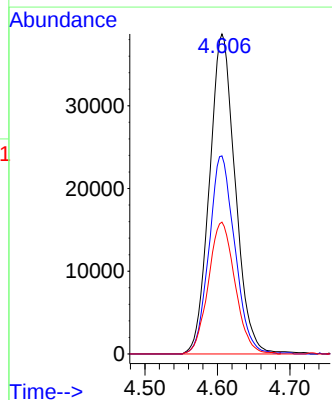
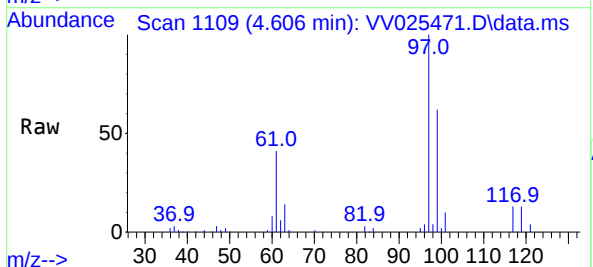




#31
Carbon tetrachloride
Concen: 6.002 ug/L
RT: 4.825 min Scan# 1176
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion:117 Resp: 83131
Ion Ratio Lower Upper
117 100
119 97.2 76.6 114.8

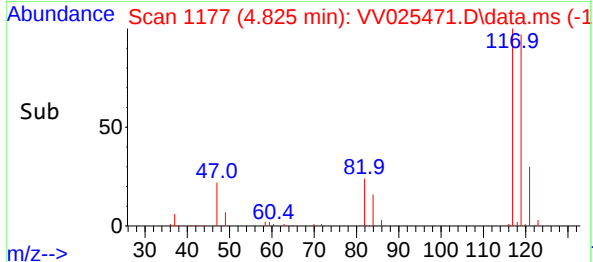

#34
Trichloroethene
Concen: 9.156 ug/L
RT: 5.912 min Scan# 1515
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 95 Resp: 99722
Ion Ratio Lower Upper
95 100
97 63.8 45.8 85.2
132 98.7 68.0 126.4
130 102.6 71.9 133.5



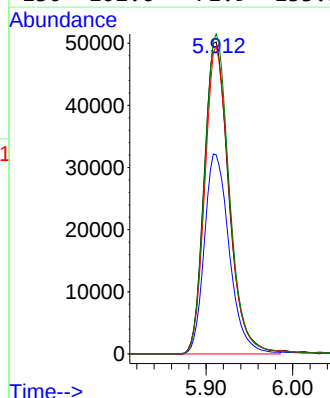





#37
1,2-Dichloropropane
Concen: 5.479 ug/L
RT: 6.172 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion: 63 Resp: 51996
Ion Ratio Lower Upper
63 100
112 5.2 3.8 5.8



#38
Bromodichloromethane
Concen: 2.371 ug/L
RT: 6.510 min Scan# 1701
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 83 Resp: 27932
Ion Ratio Lower Upper
83 100
85 61.8 44.4 82.4
127 8.4 7.2 10.8

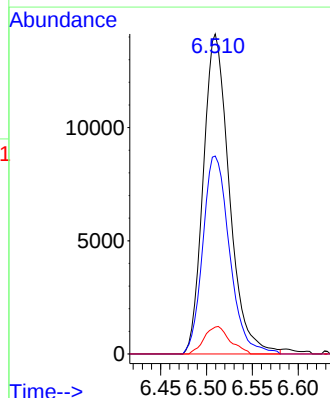



#39

cis-1,3-Dichloropropene

Concen: 1.820 ug/L

RT: 7.027 min Scan# 11

Delta R.T. 0.003 min

Lab File: VV025471.D

Acq: 12 Apr 2022 13:57

Instrument :

MSVOA_V

ClientSampleId :





GBDW5

Tgt Ion: 75 Resp: 22633

Ion Ratio Lower Upper

75 100

77 32.2 21.8 40.6

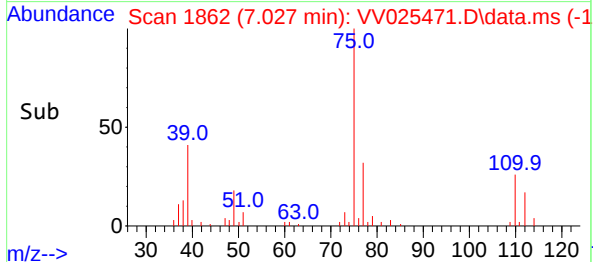

#42

Toluene

Concen: 3.261 ug/L

RT: 7.387 min Scan# 1974

Delta R.T. 0.003 min

Lab File: VV025471.D




Acq: 12 Apr 2022 13:57


Tgt Ion: 91 Resp: 145511

Ion Ratio Lower Upper

91 100

92 57.1 40.8 75.8

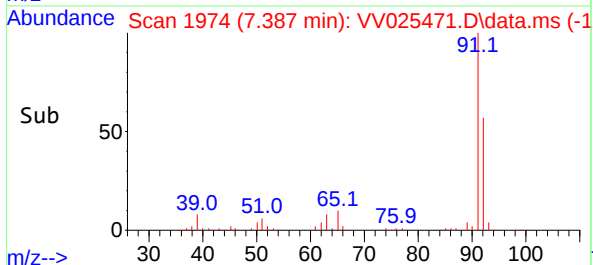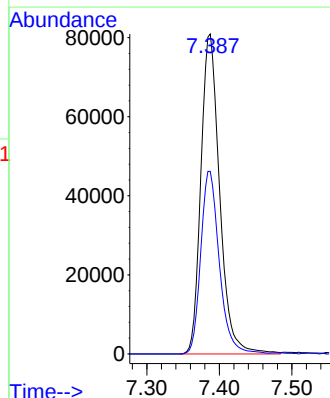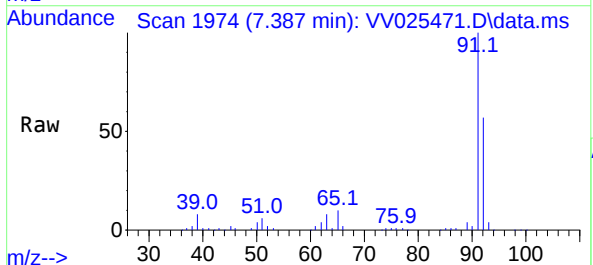







#45
1,1,2-Trichloroethane
Concen: 9.031 ug/L
RT: 7.837 min Scan# 2114
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Instrument :
MSVOA_V
ClientSampleId :
GBDW5

Tgt Ion: 97 Resp: 57391




Ion	Ratio	Lower	Upper
97	100		
99	62.4	43.8	81.4
83	86.5	60.3	112.1
85	55.4	38.7	71.9




#47
Tetrachloroethene
Concen: 5.719 ug/L
RT: 7.973 min Scan# 2156
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion: 164 Resp: 48761

Ion	Ratio	Lower	Upper
164	100		
129	94.7	66.8	124.2
131	94.5	66.4	123.4
166	123.8	91.7	170.3

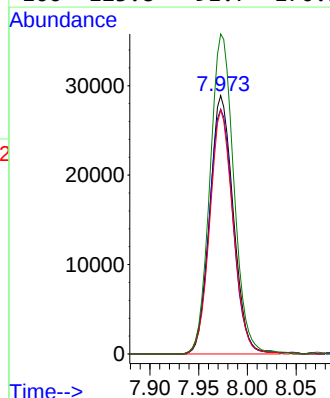



#49

Dibromochloromethane

Concen: 6.519 ug/L

RT: 8.243 min Scan# 21

Delta R.T. 0.000 min

Lab File: VV025471.D

Acq: 12 Apr 2022 13:57

Instrument :

MSVOA_V

ClientSampleId :





GBDW5

Tgt Ion:129 Resp: 45477

Ion Ratio Lower Upper

129 100

127 80.2 53.8 100.0

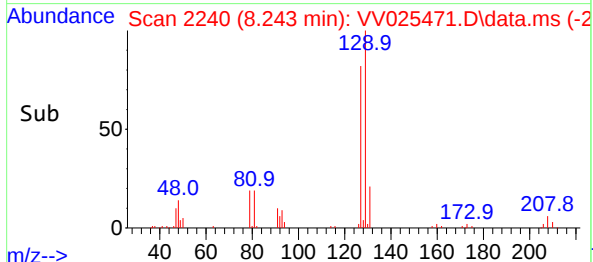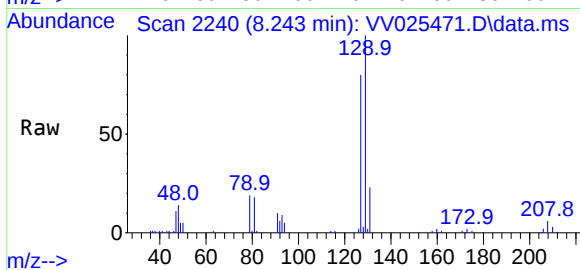

#52

Ethylbenzene

Concen: 11.479 ug/L

RT: 9.011 min Scan# 2479

Delta R.T. 0.003 min

Lab File: VV025471.D




Acq: 12 Apr 2022 13:57


Tgt Ion: 91 Resp: 546279

Ion Ratio Lower Upper

91 100

106 32.2 22.3 41.3




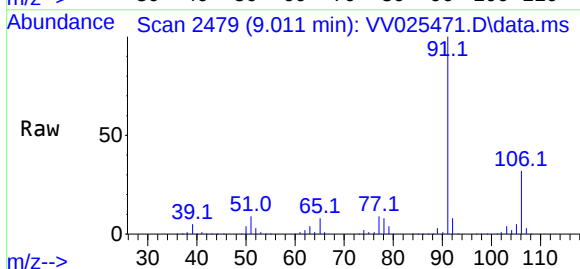




#54
o-Xylene
Concen: 3.159 ug/L
RT: 9.542 min Scan# 2644
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion:106 Resp: 55514
Ion Ratio Lower Upper
106 100
91 208.2 150.4 279.2

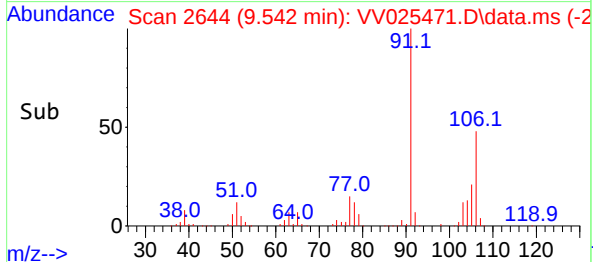

#55
Styrene
Concen: 2.896 ug/L
RT: 9.561 min Scan# 2650
Delta R.T. 0.003 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57

Tgt Ion:104 Resp: 82746
Ion Ratio Lower Upper
104 100
78 40.8 28.3 52.7

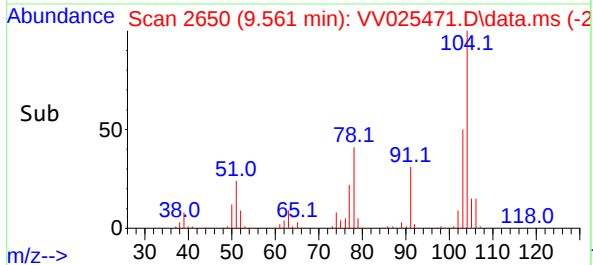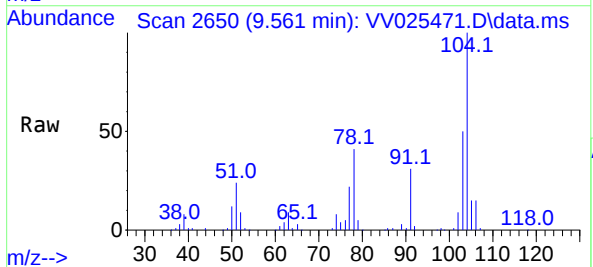

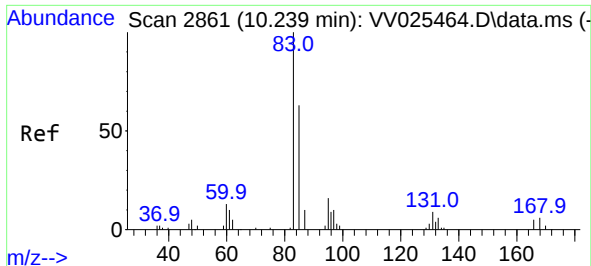

#57

1,1,2,2-Tetrachloroethane

Concen: 5.201 ug/L

RT: 10.239 min Scan# 21

Delta R.T. 0.000 min

Lab File: VV025471.D

Acq: 12 Apr 2022 13:57

Instrument :

MSVOA_V

ClientSampleId :

GBDW5





Tgt Ion: 83 Resp: 33022

Ion Ratio Lower Upper

83 100

85 65.5 45.1 83.9

131 9.5 7.9 11.9

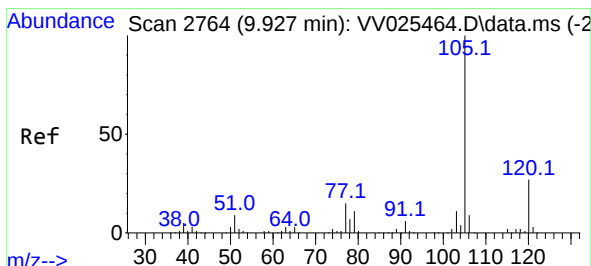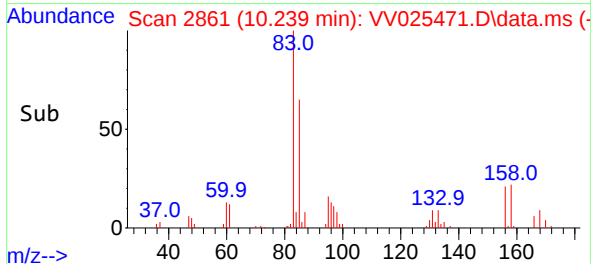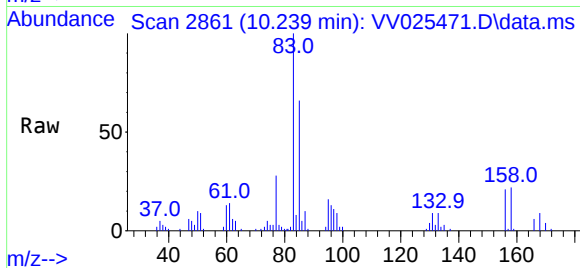

#60

Isopropylbenzene

Concen: 8.090 ug/L

RT: 9.931 min Scan# 2765

Delta R.T. 0.003 min

Lab File: VV025471.D

Acq: 12 Apr 2022 13:57




Tgt Ion: 105 Resp: 381043


Ion Ratio Lower Upper

105 100

120 26.8 21.2 31.8

77 15.1 12.2 18.2


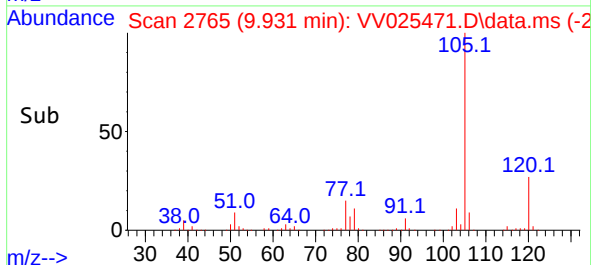
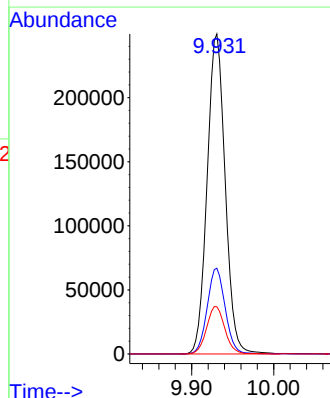
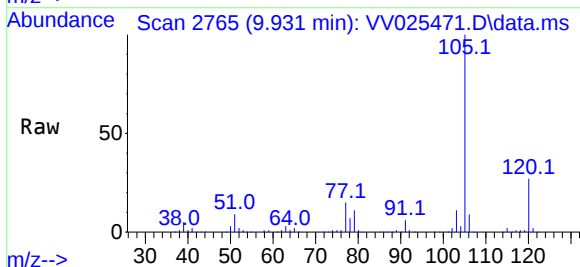


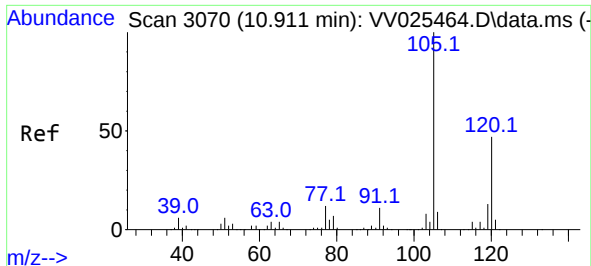

#63
1,2,4-Trimethylbenzene
Concen: 4.915 ug/L
RT: 10.911 min Scan# 3070
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57




Instrument :
MSVOA_V
ClientSampleId :
GBDW5


Tgt Ion:105 Resp: 185989
Ion Ratio Lower Upper
105 100
120 46.8 36.6 55.0

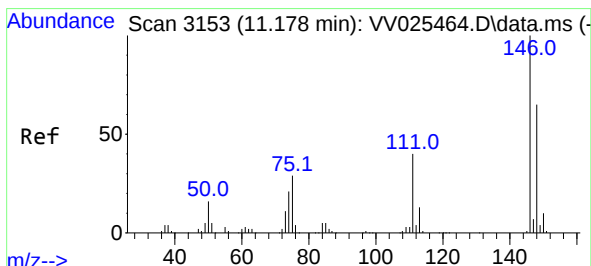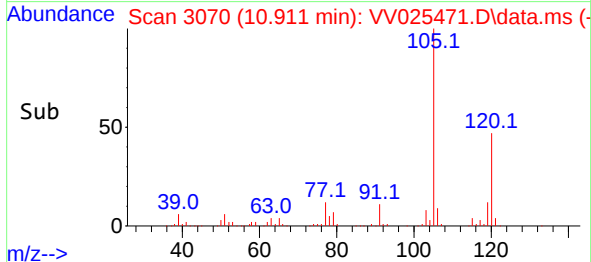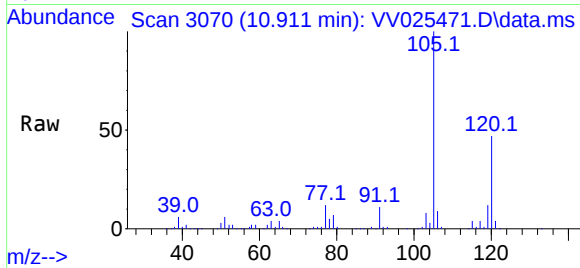

#64
1,3-Dichlorobenzene
Concen: 2.252 ug/L
RT: 11.178 min Scan# 3153
Delta R.T. 0.000 min
Lab File: VV025471.D
Acq: 12 Apr 2022 13:57


Tgt Ion:146 Resp: 49511
Ion Ratio Lower Upper
146 100
111 41.6 27.4 50.8
148 63.7 44.7 82.9

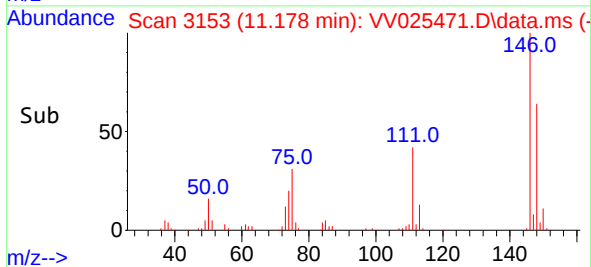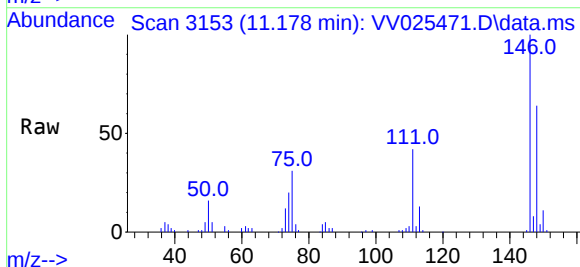

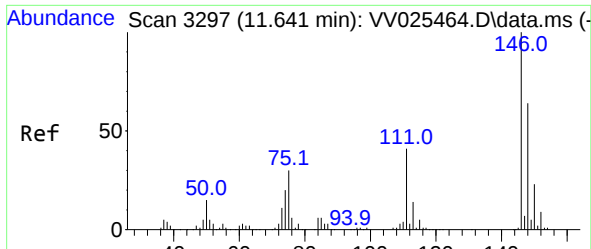

#67
 1,2-Dichlorobenzene
 Concen: 2.221 ug/L
 RT: 11.641 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV025471.D
 Acq: 12 Apr 2022 13:57

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDW5

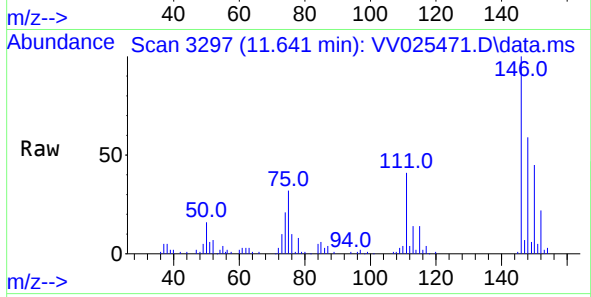

Tgt Ion:146 Resp: 43242

Ion	Ratio	Lower	Upper
146	100		
111	41.4	33.6	50.4
148	58.6	50.0	75.0

