

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025465.D
 Acq On : 12 Apr 2022 10:22
 Operator : SY/MD
 Sample : VV0412WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK340

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	101	rVB	79666	85166	20.26%	2.393%
2	1.568	156	164	176	rBV	75136	86157	20.49%	2.420%
3	2.105	321	331	354	rVB	152150	228558	54.36%	6.421%
4	2.503	447	455	468	rVB3	6178	10151	2.41%	0.285%
5	3.902	879	890	906	rBV	28712	91821	21.84%	2.580%
6	4.343	1010	1027	1053	rBV2	76108	194020	46.15%	5.451%
7	5.044	1228	1245	1279	rBV3	164154	420448	100.00%	11.812%
8	5.613	1411	1422	1447	rBV	147719	299628	71.26%	8.417%
9	5.908	1501	1514	1526	rBV5	4417	8740	2.08%	0.246%
10	6.066	1550	1563	1592	rBV2	96682	203991	48.52%	5.731%
11	6.986	1839	1849	1862	rBV2	39799	75946	18.06%	2.134%
12	7.314	1936	1951	1971	rBV	188980	339519	80.75%	9.538%
13	7.622	2038	2047	2062	rBV	22336	41635	9.90%	1.170%
14	8.088	2181	2192	2228	rBV	139008	299524	71.24%	8.415%
15	8.850	2418	2429	2456	rBV	234153	393430	93.57%	11.053%
16	10.214	2842	2853	2867	rBV2	60268	98458	23.42%	2.766%
17	11.246	3164	3174	3191	rBV	238262	375149	89.23%	10.539%
18	11.622	3280	3291	3310	rBV	184631	293857	69.89%	8.255%
19	12.249	3477	3486	3497	rBV	3146	4626	1.10%	0.130%
20	13.506	3869	3877	3885	rBV3	2662	4351	1.03%	0.122%
21	13.744	3941	3951	3960	rBV6	2736	4422	1.05%	0.124%




Sum of corrected areas: 3559597

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025465.D
Acq On : 12 Apr 2022 10:22
Operator : SY/MD
Sample : VV0412WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK340

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

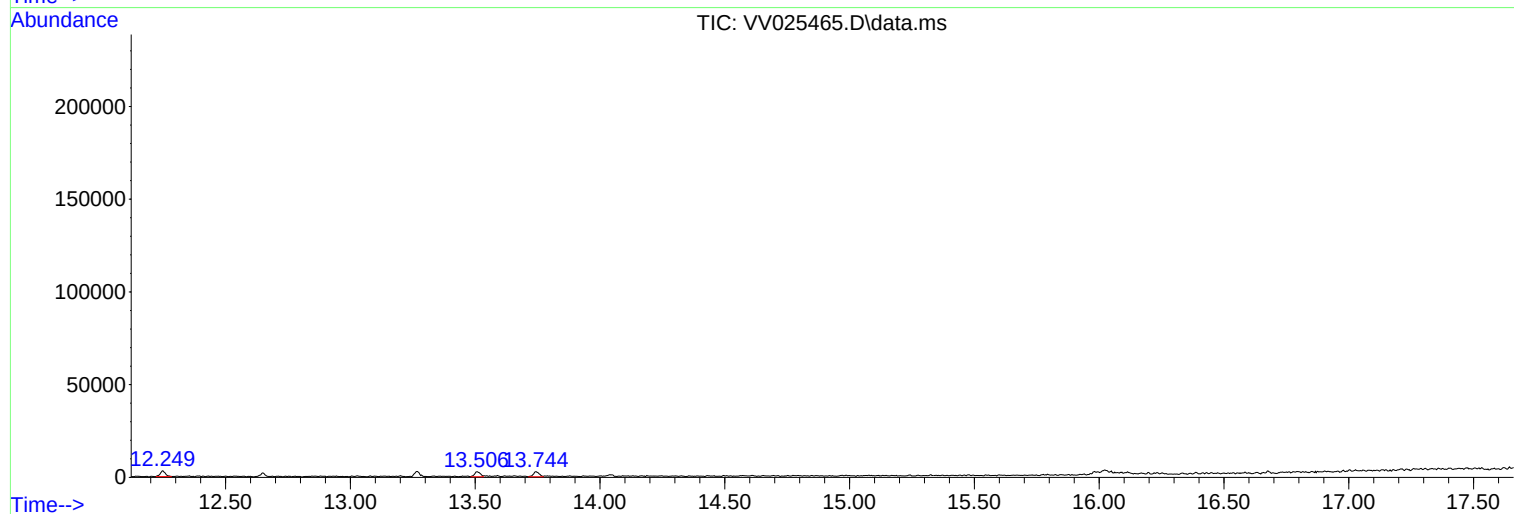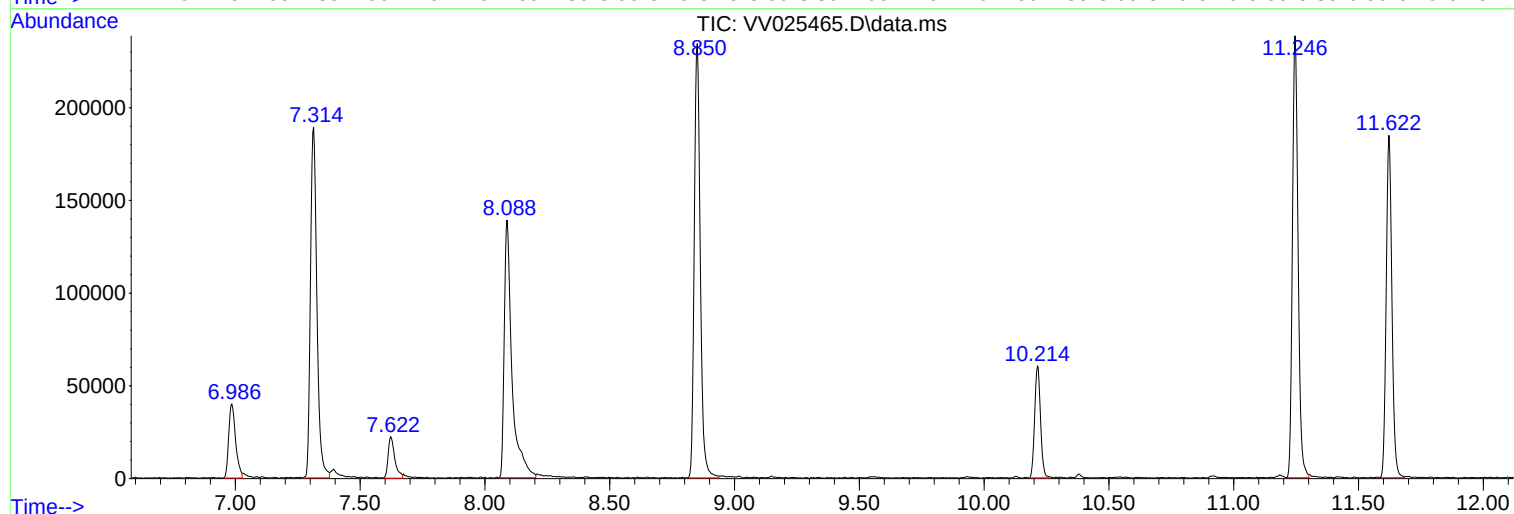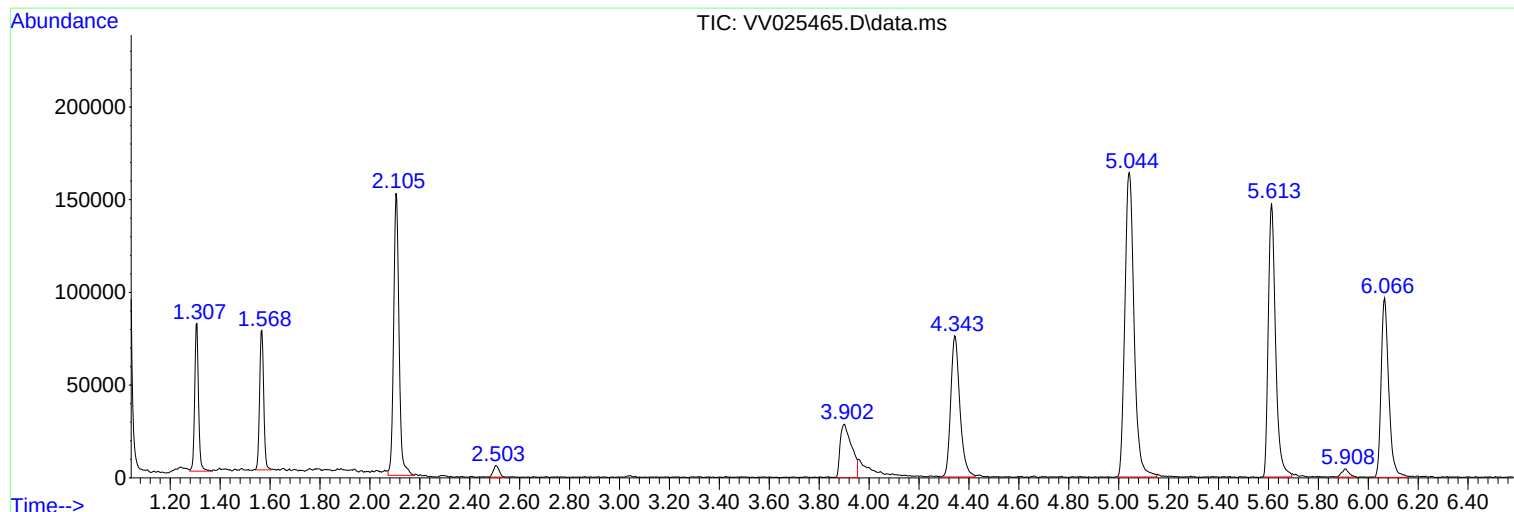

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025465.D
Acq On : 12 Apr 2022 10:22
Operator : SY/MD
Sample : VV0412WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK340

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025465.D
Acq On : 12 Apr 2022 10:22
Operator : SY/MD
Sample : VV0412WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK340

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
