

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025470.D
 Acq On : 12 Apr 2022 12:34
 Operator : SY/MD
 Sample : VIBLK244
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK244

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	94	rBV	71977	78518	21.04%	2.717%
2	1.568	157	164	176	rBV	74343	85900	23.02%	2.972%
3	2.108	323	332	351	rVB	110155	166639	44.65%	5.766%
4	2.510	447	457	470	rVB3	5214	8807	2.36%	0.305%
5	3.895	878	888	925	rBV2	43192	144277	38.66%	4.992%
6	4.352	1015	1030	1054	rBV	70713	177111	47.45%	6.128%
7	5.050	1231	1247	1277	rBV3	145607	373227	100.00%	12.914%
8	5.619	1414	1424	1444	rBV2	88040	180010	48.23%	6.228%
9	5.915	1507	1516	1532	rVB7	5904	13540	3.63%	0.468%
10	6.072	1550	1565	1586	rBV2	92333	192941	51.70%	6.676%
11	6.989	1840	1850	1868	rBV2	33364	64659	17.32%	2.237%
12	7.317	1939	1952	1974	rBV	136738	244176	65.42%	8.449%
13	7.628	2036	2049	2072	rBV2	19632	38877	10.42%	1.345%
14	7.979	2151	2158	2170	rVB3	7228	12706	3.40%	0.440%
15	8.091	2182	2193	2226	rBV	172358	358988	96.18%	12.421%
16	8.853	2418	2430	2452	rBV	138065	226275	60.63%	7.829%
17	10.217	2843	2854	2870	rBV	66469	105960	28.39%	3.666%
18	10.384	2897	2906	2917	rBV3	3313	5200	1.39%	0.180%
19	11.249	3164	3175	3193	rBV	124801	195604	52.41%	6.768%
20	11.622	3281	3291	3306	rBV	128176	202324	54.21%	7.000%
21	16.178	4698	4708	4716	rBV5	9438	14411	3.86%	0.499%




Sum of corrected areas: 2890150

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025470.D
Acq On : 12 Apr 2022 12:34
Operator : SY/MD
Sample : VIBLK244
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

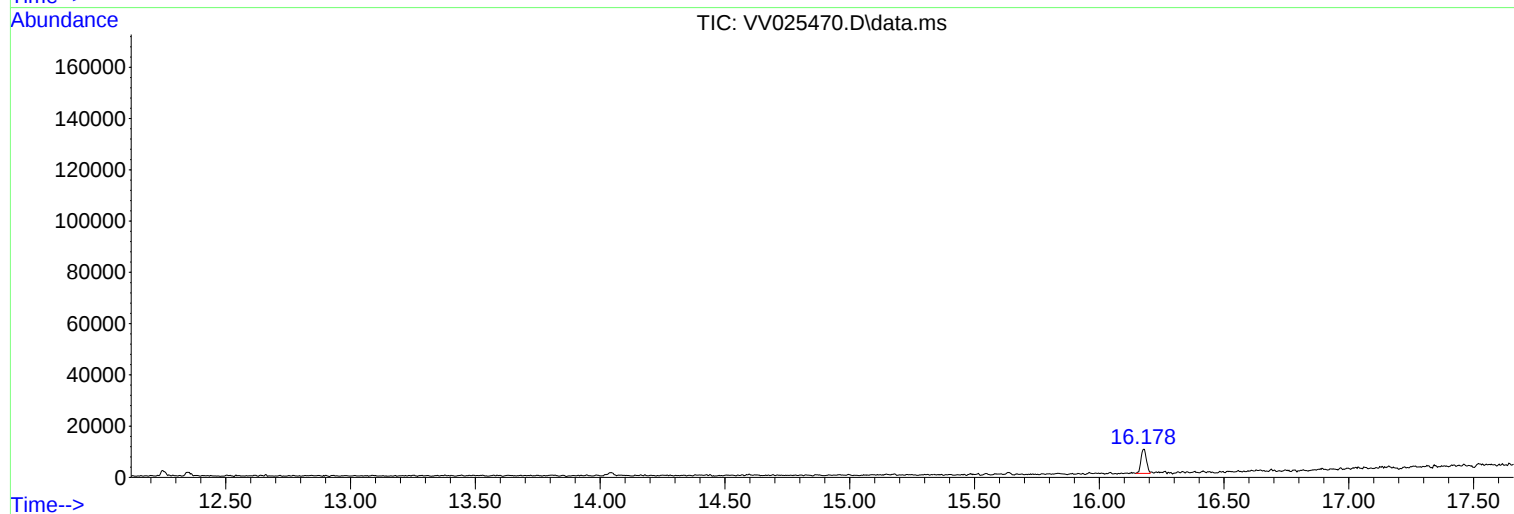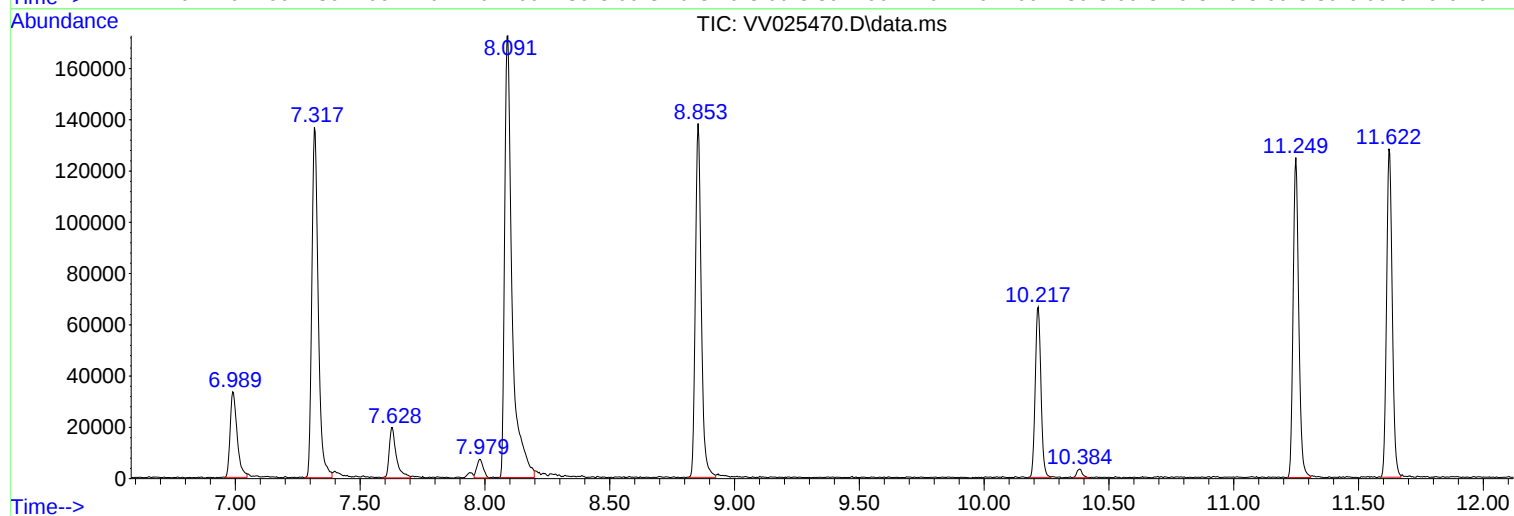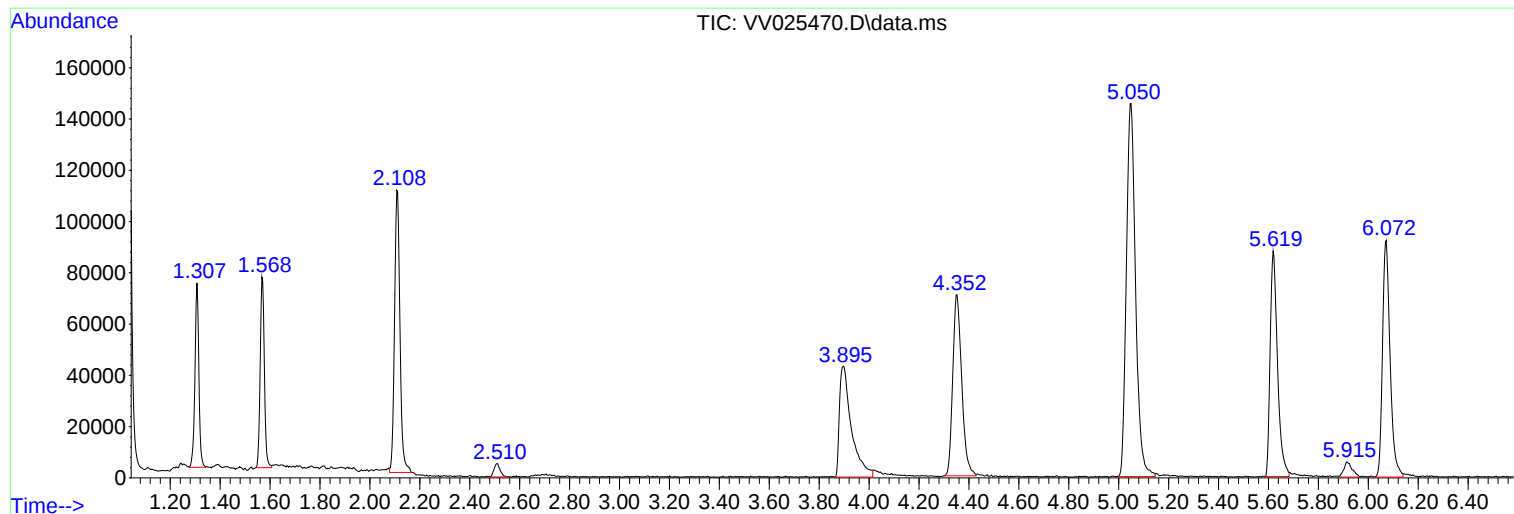

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025470.D
Acq On : 12 Apr 2022 12:34
Operator : SY/MD
Sample : VIBLK244
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025470.D
Acq On : 12 Apr 2022 12:34
Operator : SY/MD
Sample : VIBLK244
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc