

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
 Data File : VV025478.D
 Acq On : 12 Apr 2022 16:42
 Operator : SY/MD
 Sample : N2356-23
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDW3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	49	63	74	rBV3	4319	8590	1.98%	0.233%
2	1.310	76	84	96	rVB	74825	75641	17.40%	2.050%
3	1.571	157	165	173	rBV	73875	82729	19.03%	2.242%
4	2.111	322	333	353	rVB	142229	209323	48.16%	5.673%
5	3.905	881	891	892	rBV	34575	40361	9.29%	1.094%
6	4.352	1013	1030	1065	rBV	79032	202691	46.64%	5.493%
7	5.050	1232	1247	1268	rBV3	174471	430615	99.08%	11.670%
8	5.619	1413	1424	1446	rBV	161723	331698	76.32%	8.989%
9	5.915	1507	1516	1530	rBV6	4175	9318	2.14%	0.253%
10	6.072	1550	1565	1592	rBV2	100114	213342	49.09%	5.782%
11	6.992	1839	1851	1865	rBV2	40589	77209	17.76%	2.092%
12	7.317	1940	1952	1971	rBV	194035	346969	79.83%	9.403%
13	7.625	2038	2048	2068	rBV2	21735	42193	9.71%	1.143%
14	8.091	2183	2193	2235	rBV	163821	352066	81.00%	9.541%
15	8.853	2419	2430	2451	rBV	261050	434629	100.00%	11.778%
16	10.217	2840	2854	2871	rBV2	67669	110068	25.32%	2.983%
17	10.381	2897	2905	2913	rBV4	2864	4514	1.04%	0.122%
18	11.249	3164	3175	3199	rBV	252580	399728	91.97%	10.833%
19	11.622	3280	3291	3308	rBV	188819	301807	69.44%	8.179%
20	12.348	3506	3517	3524	rBV7	4555	6871	1.58%	0.186%
21	13.435	3846	3855	3865	rBV4	6753	9667	2.22%	0.262%


Sum of corrected areas: 3690029

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025478.D
Acq On : 12 Apr 2022 16:42
Operator : SY/MD
Sample : N2356-23
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

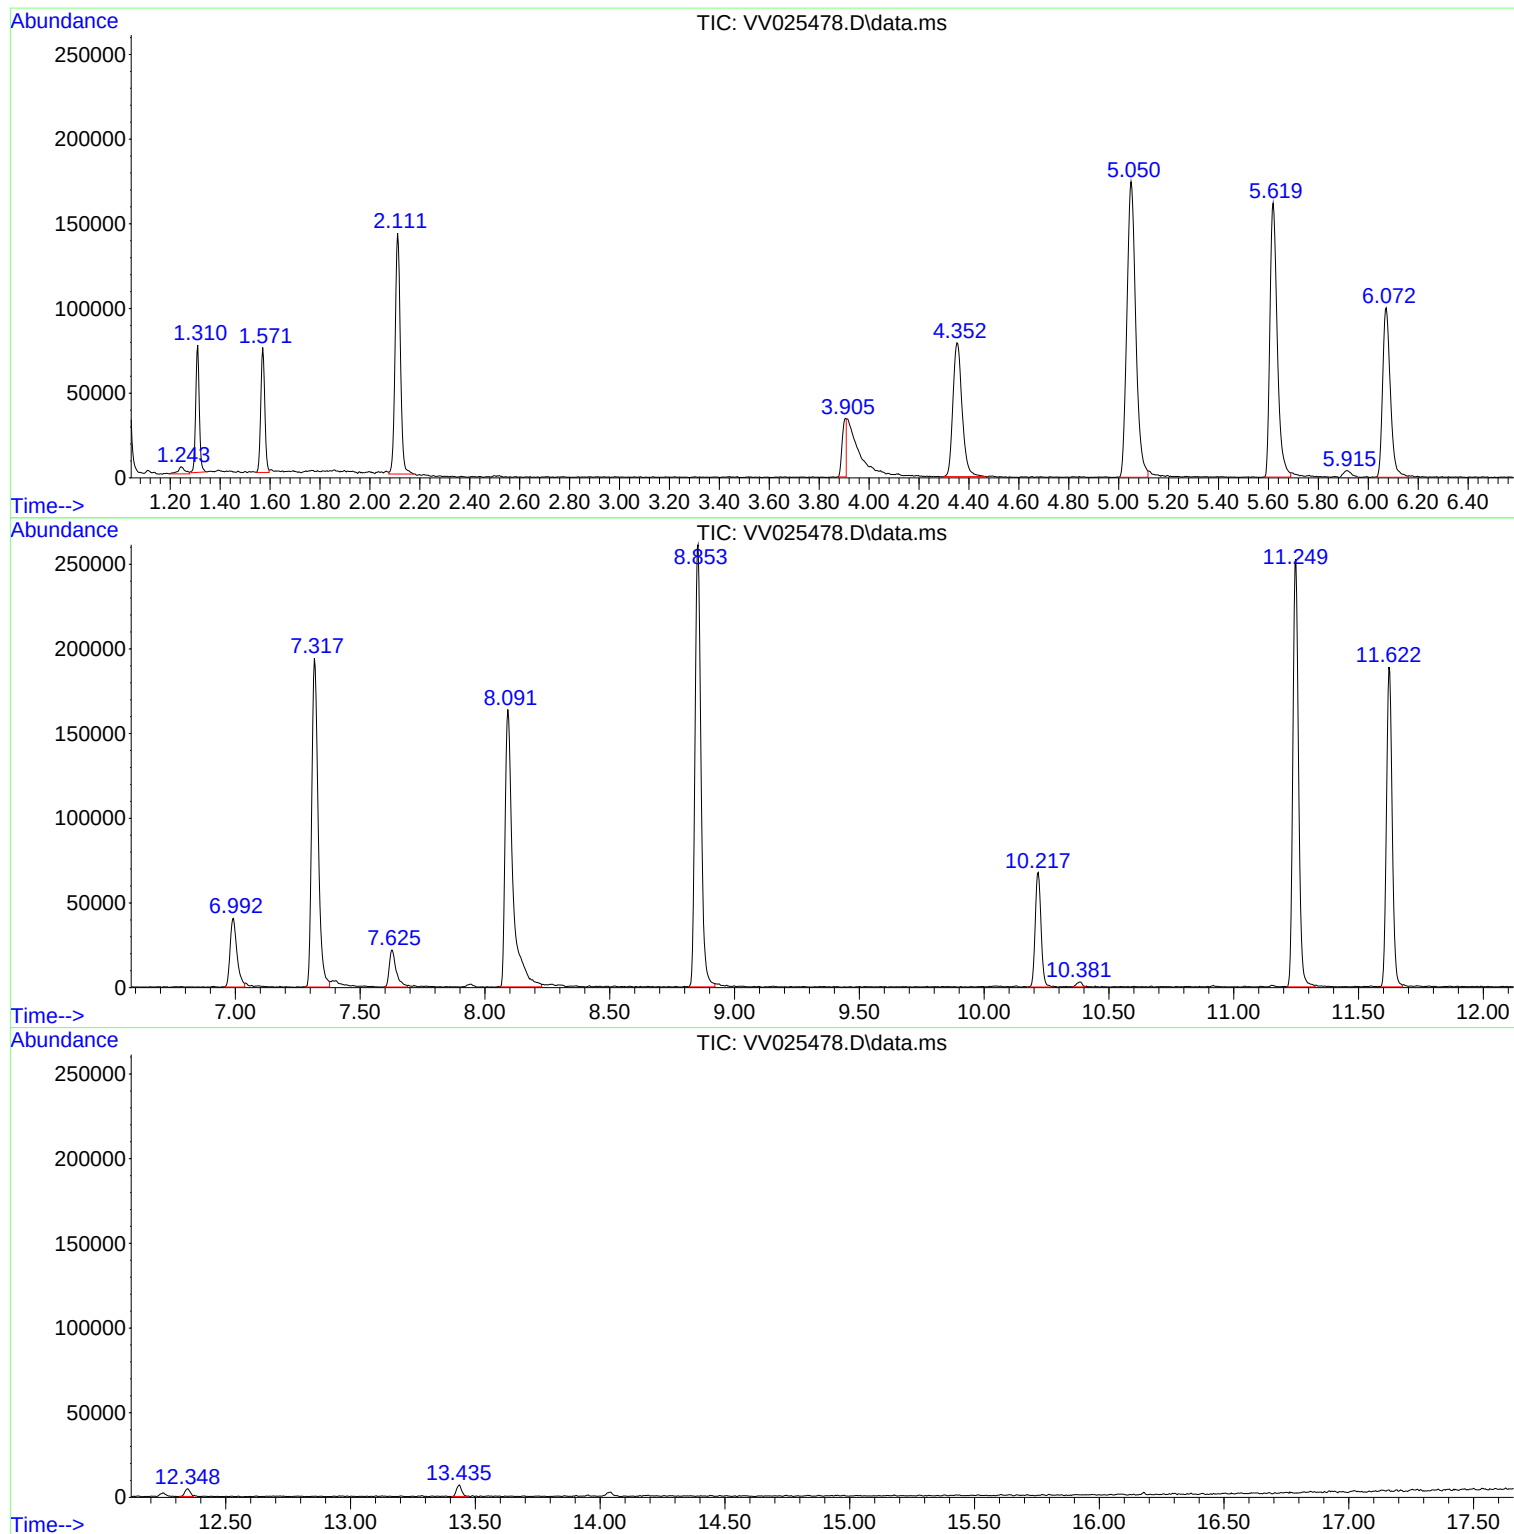

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025478.D
Acq On : 12 Apr 2022 16:42
Operator : SY/MD
Sample : N2356-23
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025478.D
Acq On : 12 Apr 2022 16:42
Operator : SY/MD
Sample : N2356-23
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc