
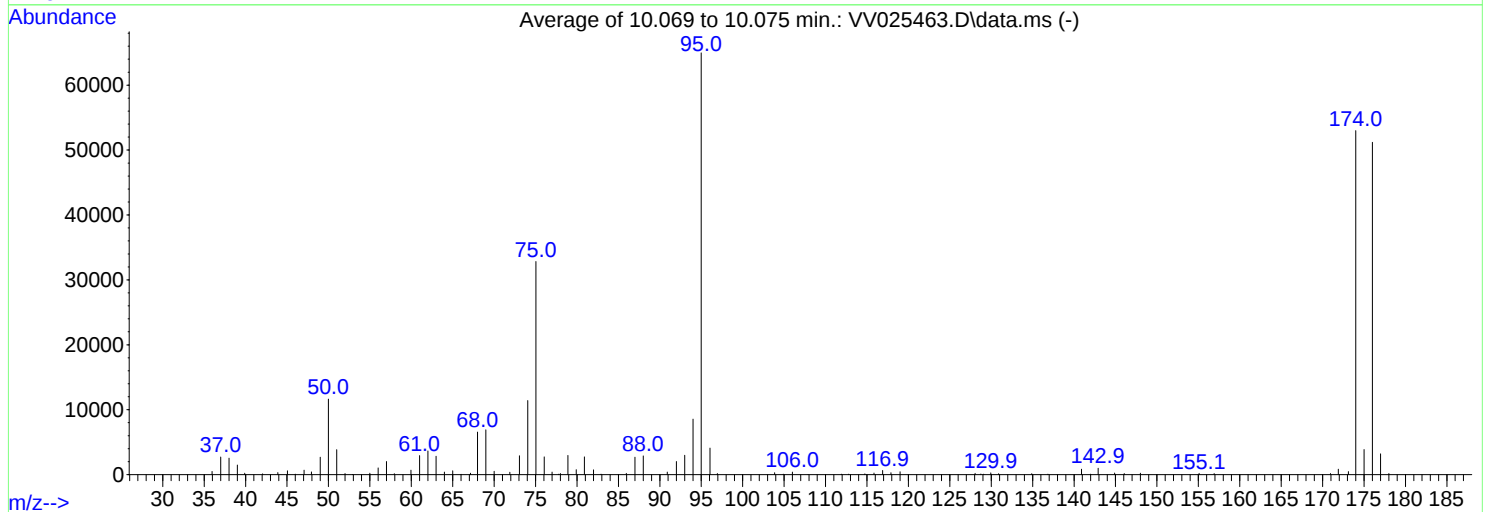


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041222\
Data File : VV025463.D
Acq On : 12 Apr 2022 09:05
Operator : SY/MD
Sample : BFB300
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB300

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 13 02:31:13 2022

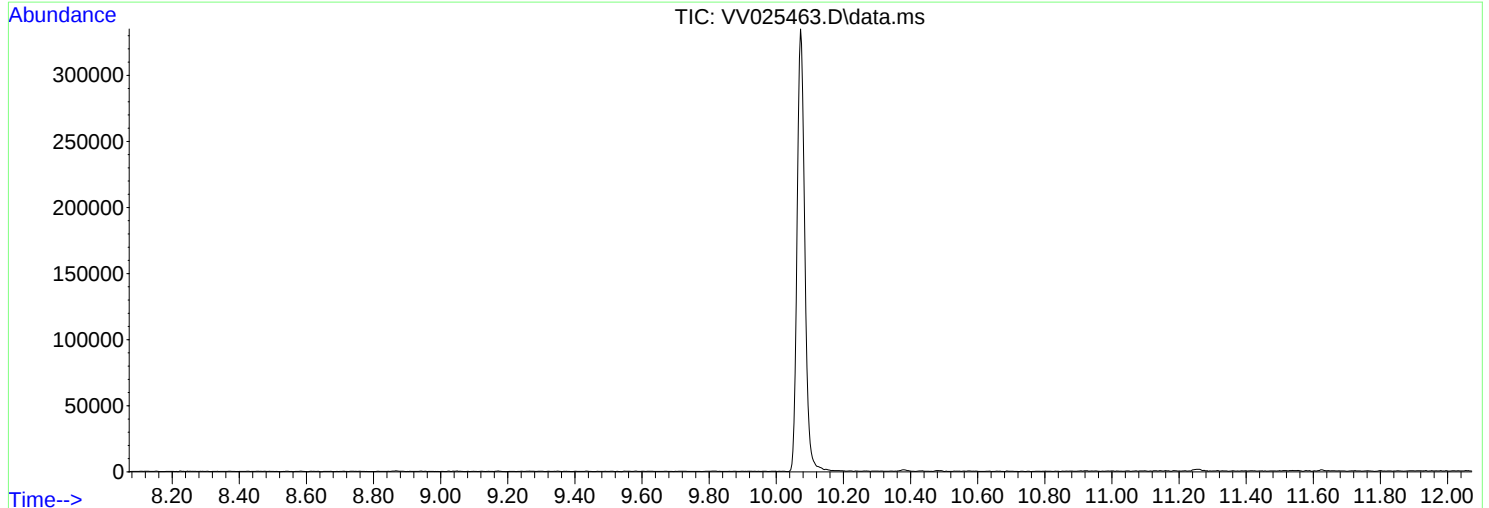

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	11634	PASS
75	95	30	80	50.5	32821	PASS
95	95	100	100	100.0	64976	PASS
96	95	5	9	6.3	4084	PASS
173	174	0.00	2	0.9	479	PASS
174	95	50	120	81.6	52992	PASS
175	174	5	9	7.3	3877	PASS
176	174	95	105	96.6	51205	PASS
177	176	5	10	6.3	3204	PASS

m/z	Abundance
43.90	315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
35.90	566.0
37.00	2745.0
38.00	2338.0
39.00	1351.0
39.90	203.0
42.10	114.0
43.90	633.0
45.00	595.0
46.00	132.0
47.00	612.0
47.90	446.0
49.00	2540.0
50.00	11642.0
51.00	3744.0
52.00	166.0
52.90	113.0
54.90	231.0
56.00	972.0
57.00	2095.0
58.00	138.0
60.00	667.0
61.00	2969.0
62.00	3660.0
63.00	2701.0
64.00	452.0
65.00	586.0
66.00	126.0
67.20	243.0
68.00	6251.0
69.00	6606.0
70.00	521.0
71.90	342.0
73.10	2915.0
74.00	10924.0
75.10	31832.0
76.00	2824.0
77.00	411.0
77.80	225.0
78.90	2782.0
79.90	732.0
80.90	2577.0
82.00	727.0
86.00	212.0
87.00	2728.0
88.00	2926.0
90.90	352.0
92.00	2004.0
93.00	2846.0
94.00	8163.0
95.00	63408.0
96.00	4120.0
96.90	149.0
103.80	316.0
106.00	389.0
114.80	124.0
115.90	214.0
116.90	577.0
117.90	303.0
119.00	449.0
128.00	209.0
128.80	100.0
130.00	291.0
130.90	124.0
134.90	155.0
136.90	127.0
140.90	820.0
142.00	113.0
142.90	914.0
144.90	244.0
146.00	175.0
148.00	193.0
155.10	153.0
156.90	138.0
170.90	166.0
171.90	786.0
173.10	701.0
174.00	50744.0
175.00	3587.0
176.00	48296.0
177.00	2919.0
178.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
35.90	501.0
37.00	2809.0
38.00	2598.0
39.00	1538.0
39.90	233.0
42.00	117.0
44.00	629.0
45.10	594.0
46.00	106.0
47.00	764.0
47.90	408.0
49.00	2761.0
50.00	12025.0
51.00	4018.0
52.00	181.0
55.00	208.0
56.00	1058.0
57.00	2094.0
57.90	136.0
59.90	709.0
61.00	3020.0
62.00	3831.0
63.00	2949.0
64.00	407.0
65.00	617.0
67.10	231.0
68.00	6764.0
69.00	7117.0
70.00	516.0
71.90	399.0
73.00	3004.0
74.00	11771.0
75.10	33888.0
76.10	2859.0
77.00	402.0
78.00	254.0
78.90	3055.0
79.90	790.0
80.90	2816.0
82.00	769.0
82.90	112.0
85.90	216.0
87.00	2741.0
88.00	3003.0
90.90	411.0
92.00	2062.0
93.00	3072.0
94.00	8949.0
95.00	67352.0
96.00	4236.0
97.00	173.0
103.80	316.0
104.90	105.0
106.00	420.0
111.90	106.0
112.80	105.0
114.70	120.0
115.80	254.0
116.90	685.0
117.90	307.0
119.00	438.0
128.00	210.0
128.70	103.0
129.10	117.0
129.90	288.0
130.90	155.0
134.90	162.0
136.80	108.0
140.90	850.0
142.00	102.0
142.90	1010.0
144.90	251.0
146.10	173.0
148.00	239.0
155.10	199.0
156.90	170.0
171.00	186.0
171.90	872.0
173.10	735.0
174.00	54720.0
175.00	3969.0
176.00	52808.0
177.00	3288.0
178.00	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300

m/z	Abundance
36.00	422.0
37.00	2598.0
38.00	2664.0
39.00	1543.0
39.90	206.0
42.00	111.0
44.00	625.0
45.00	563.0
47.10	721.0
48.00	371.0
49.00	2785.0
50.00	11235.0
51.00	3816.0
52.00	187.0
55.10	209.0
56.00	1070.0
57.00	1887.0
57.90	150.0
59.90	667.0
61.00	2847.0
62.00	3477.0
63.00	2828.0
64.00	337.0
65.00	614.0
67.10	212.0
68.00	6680.0
69.00	7009.0
70.00	498.0
71.90	407.0
73.00	2814.0
74.10	11577.0
75.00	32744.0
76.00	2542.0
77.00	359.0
78.00	292.0
78.90	3015.0
79.90	753.0
80.90	2856.0
82.00	743.0
82.90	119.0
86.00	181.0
87.00	2568.0
88.00	2731.0
90.90	391.0
92.00	1975.0
93.00	3034.0
94.00	8554.0
95.00	64168.0
96.10	3897.0
97.00	169.0
103.90	267.0
104.90	123.0
106.00	411.0
107.90	104.0
111.90	109.0
112.80	104.0
114.70	122.0
115.80	298.0
116.90	701.0
117.90	304.0
119.00	425.0
128.10	193.0
128.70	109.0
129.10	121.0
129.90	280.0
130.90	151.0
134.90	168.0
140.90	846.0
142.90	1007.0
144.90	273.0
146.10	148.0
148.00	222.0
150.00	114.0
155.10	217.0
156.90	192.0
171.00	157.0
171.90	874.0
174.00	53512.0
175.00	4076.0
176.00	52512.0
177.00	3405.0
178.00	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB300