

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025491.D
 Acq On : 13 Apr 2022 13:39
 Operator : SY/MD
 Sample : N2319-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 14 03:10:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 03:09:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	159889	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	162516	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77776	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	77350	5.203	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	104.000%	
7) Chloroethane-d5	1.571	69	65912	4.168	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.400%	
11) 1,1-Dichloroethene-d2	2.111	63	117130	3.933	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.600%	
20) 2-Butanone-d5	3.908	46	79257	43.832	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.660%	
24) Chloroform-d	4.352	84	104095	4.634	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.600%	
26) 1,2-Dichloroethane-d4	5.037	65	48358	4.996	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.000%	
32) Benzene-d6	5.053	84	216941	4.614	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
36) 1,2-Dichloropropane-d6	6.069	67	62054	4.732	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.600%	
41) Toluene-d8	7.317	98	186572	4.276	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.625	79	17672	4.009	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.200%	
46) 2-Hexanone-d5	8.088	63	61360	39.664	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	79.320%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35036	4.229	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	84.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	62771	4.814	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.200%	
Target Compounds					Qvalue	
25) Chloroform	4.378	83	2680	0.129	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025491.D
Acq On : 13 Apr 2022 13:39
Operator : SY/MD
Sample : N2319-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Apr 14 03:10:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 03:09:10 2022
Response via : Initial Calibration

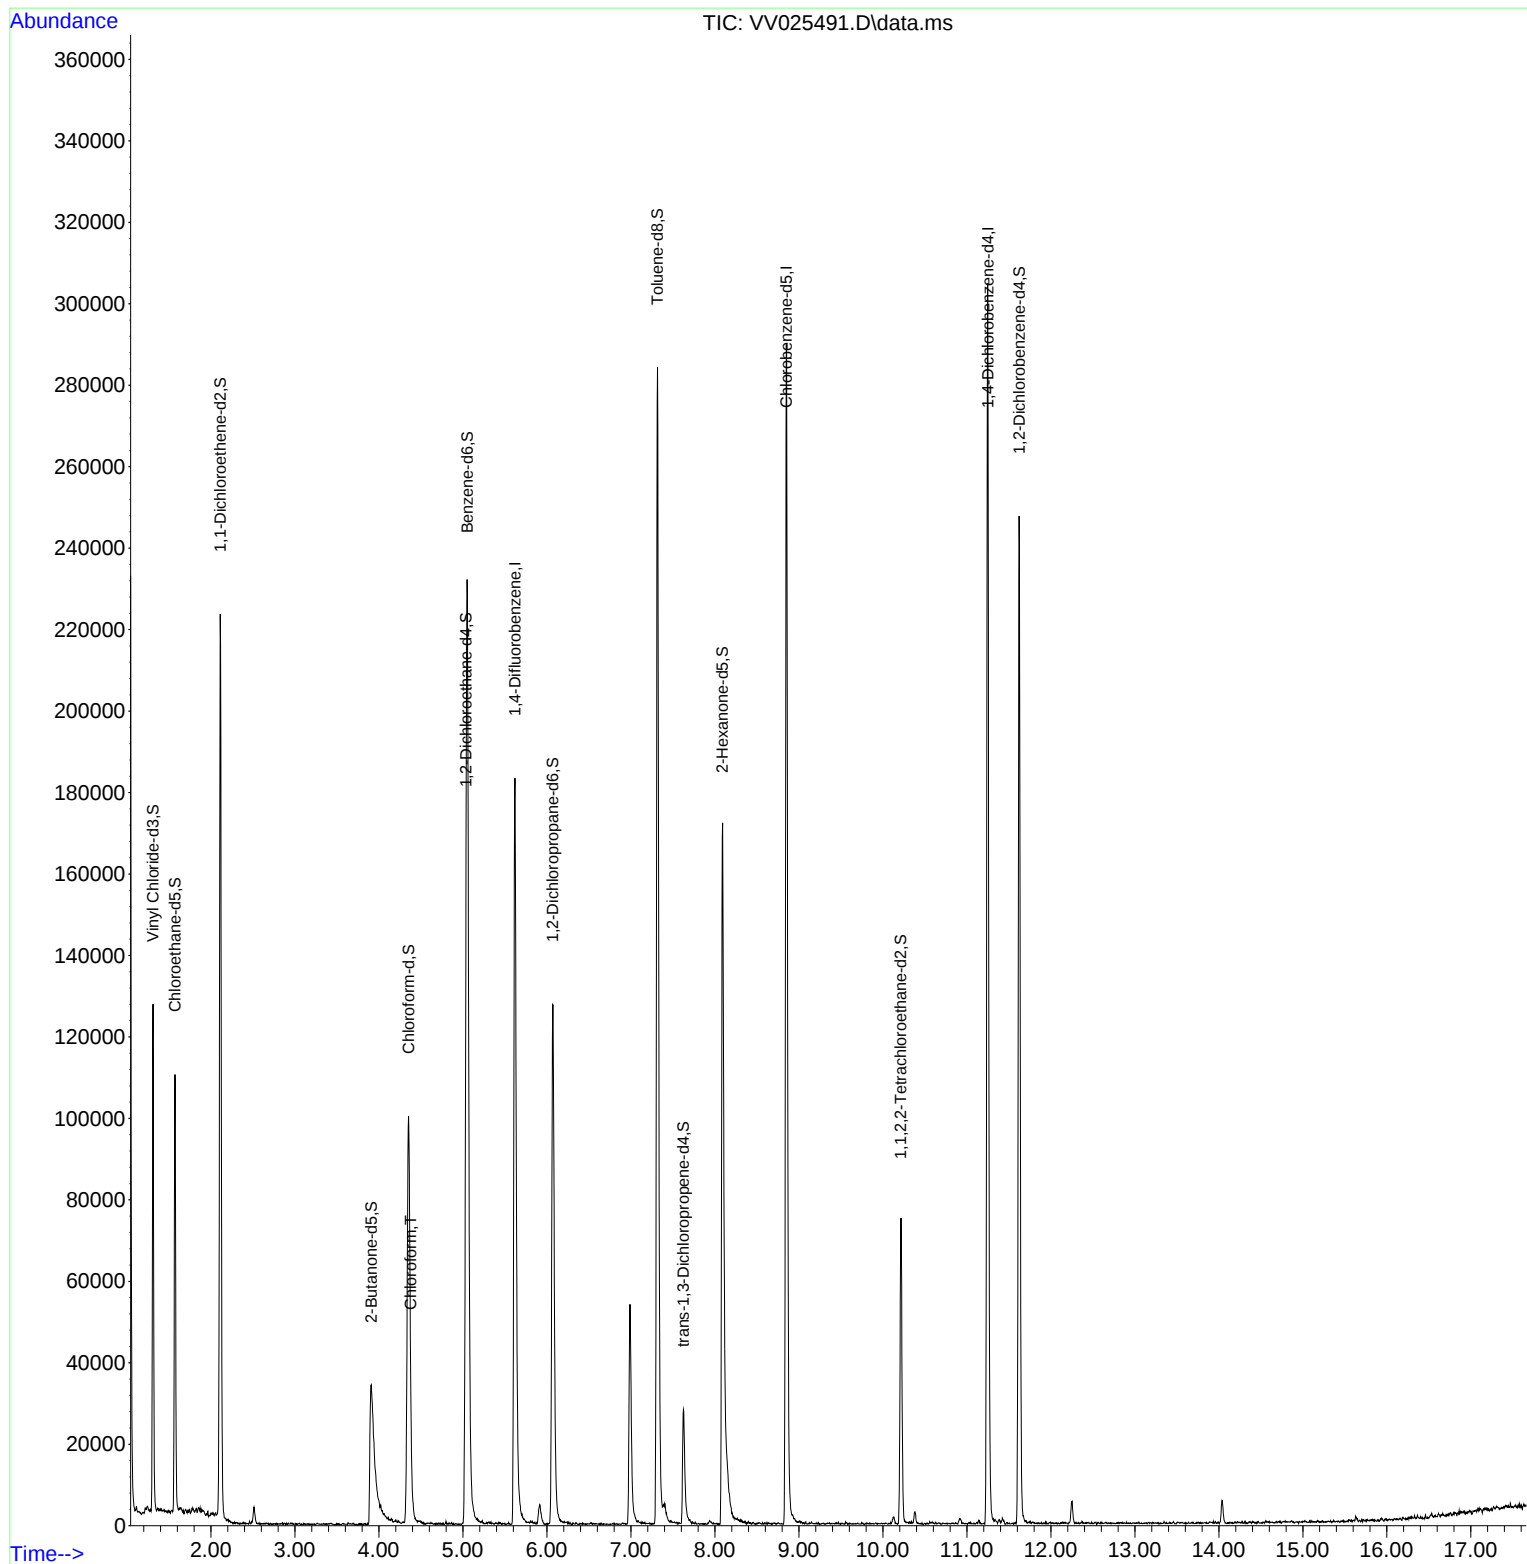

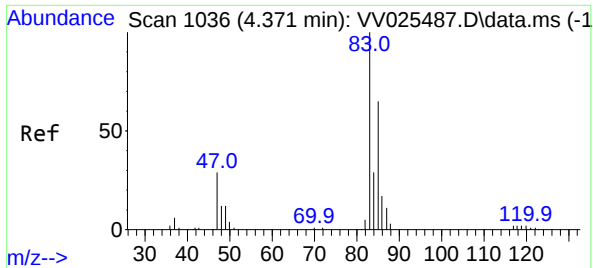

#25
Chloroform
Concen: 0.129 ug/L
RT: 4.378 min Scan# 10
Delta R.T. 0.006 min
Lab File: VV025491.D
Acq: 13 Apr 2022 13:39

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 83 Resp: 2680
Ion Ratio Lower Upper
83 100
85 63.0 43.5 80.7

