

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025493.D
 Acq On : 13 Apr 2022 15:36
 Operator : SY/MD
 Sample : N2373-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFD6

Quant Time: Apr 14 03:10:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 03:09:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	150719	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	152296	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	71454	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	88078	6.286	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	125.800%
7) Chloroethane-d5	1.571	69	74935	5.027	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.600%
11) 1,1-Dichloroethene-d2	2.111	63	130040	4.633	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	92.600%
20) 2-Butanone-d5	3.892	46	92300	54.151	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.300%
24) Chloroform-d	4.346	84	118329	5.588	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.800%
26) 1,2-Dichloroethane-d4	5.027	65	54775	6.004	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.000%
32) Benzene-d6	5.047	84	243028	5.515	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.400%
36) 1,2-Dichloropropane-d6	6.063	67	68832	5.601	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.000%
41) Toluene-d8	7.310	98	210834	5.156	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
43) trans-1,3-Dichloroprop...	7.622	79	19293	4.671	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.400%
46) 2-Hexanone-d5	8.085	63	66880	46.134	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.260%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37637	4.848	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	68324	5.703	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.000%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	2996	0.236	ug/L	90
25) Chloroform	4.378	83	13707	0.700	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025493.D
Acq On : 13 Apr 2022 15:36
Operator : SY/MD
Sample : N2373-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFD6

Quant Time: Apr 14 03:10:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 03:09:10 2022
Response via : Initial Calibration




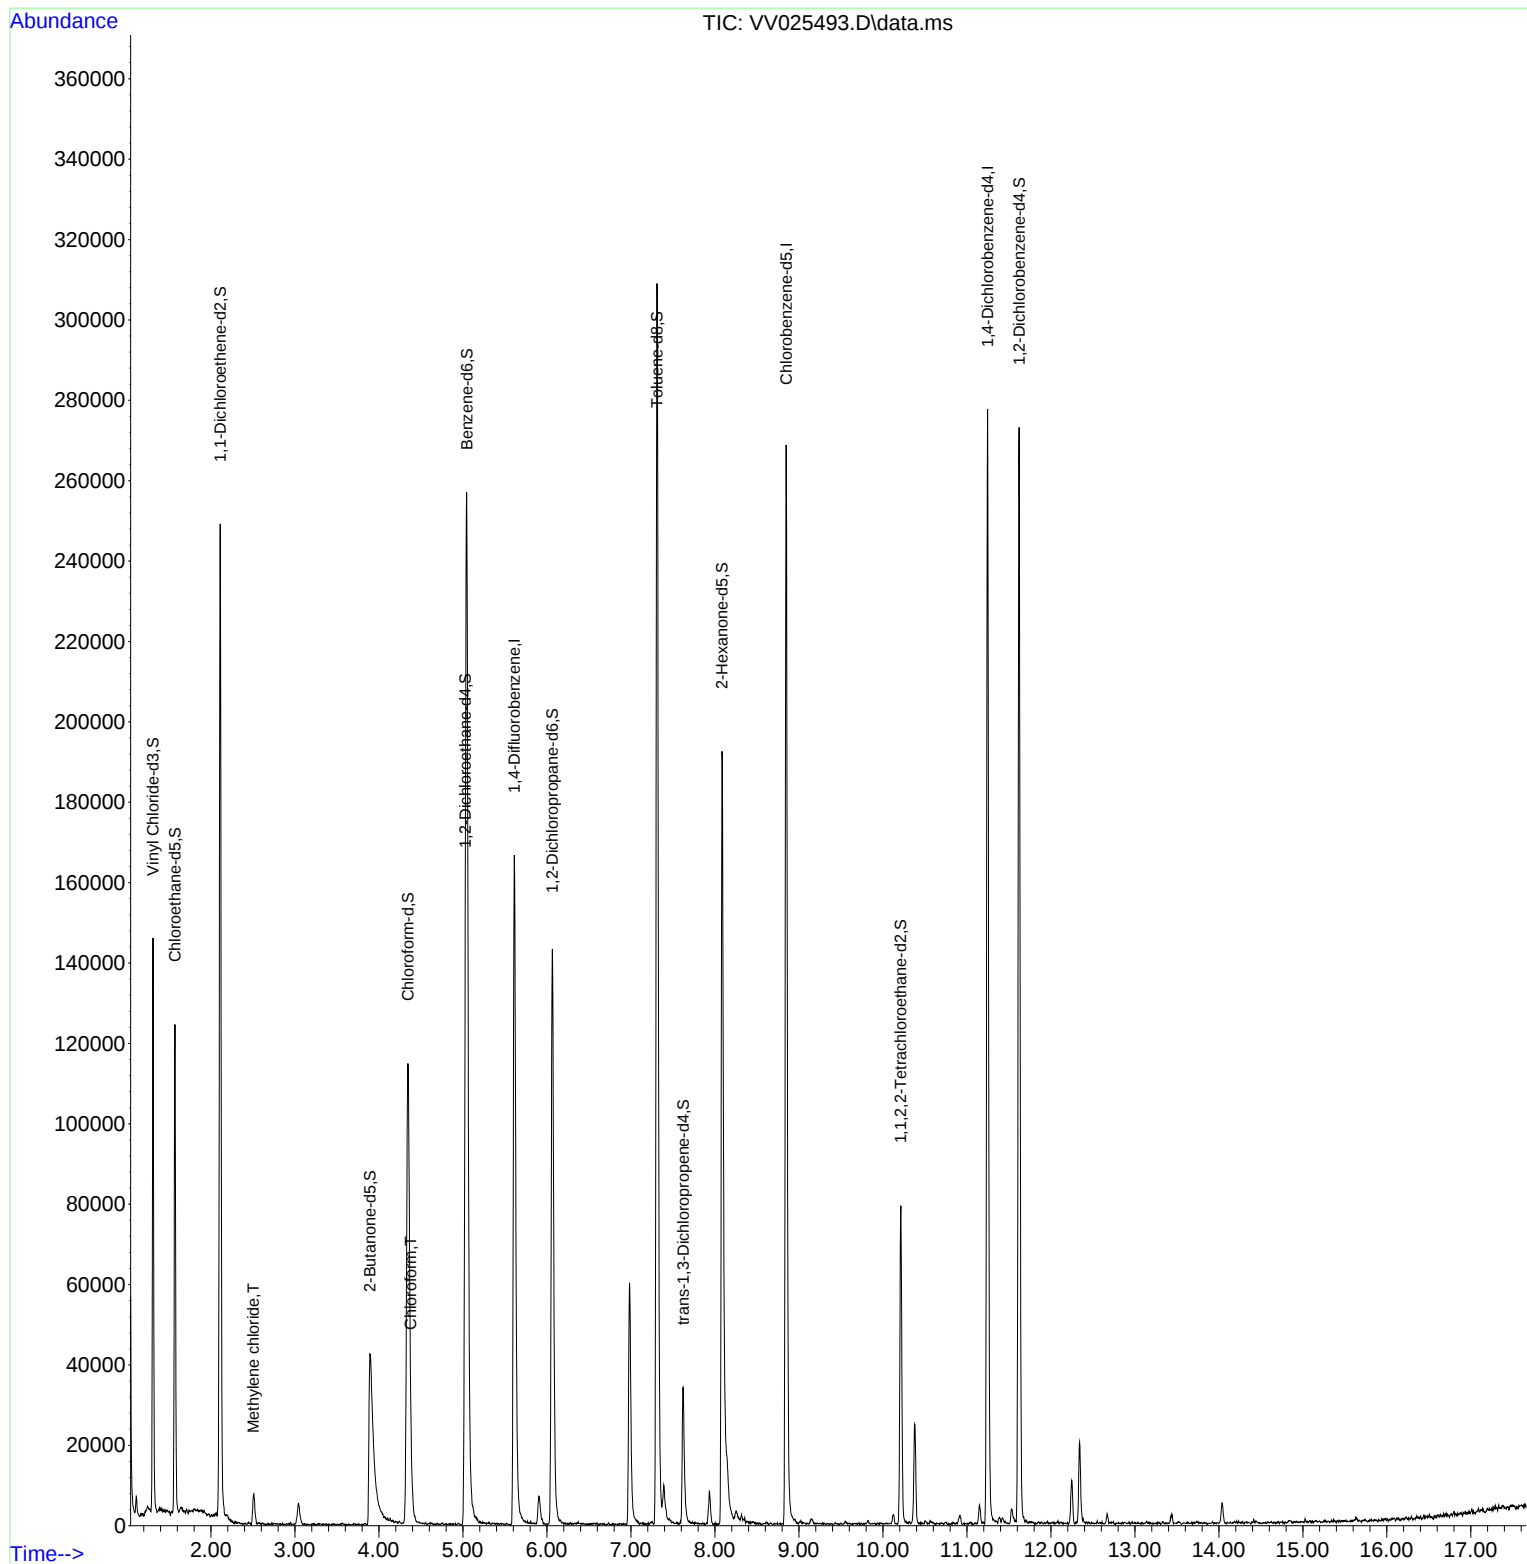


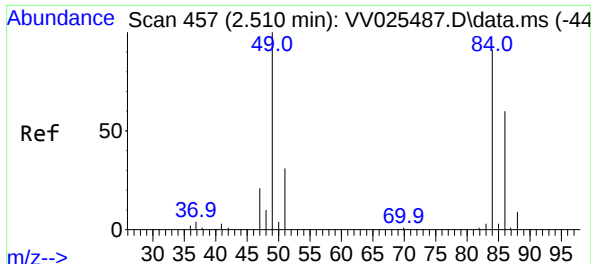

#16
Methylene chloride
Concen: 0.236 ug/L
RT: 2.507 min Scan# 41
Delta R.T. -0.003 min
Lab File: VV025493.D
Acq: 13 Apr 2022 15:36

Instrument :
MSVOA_V
ClientSampleId :
BFFD6

Tgt Ion: 84 Resp: 2996
Ion Ratio Lower Upper
84 100
86 55.8 45.9 85.3
49 118.9 76.6 142.3

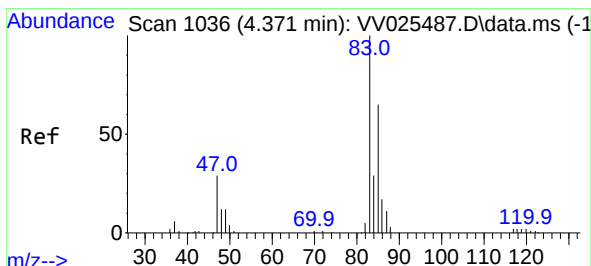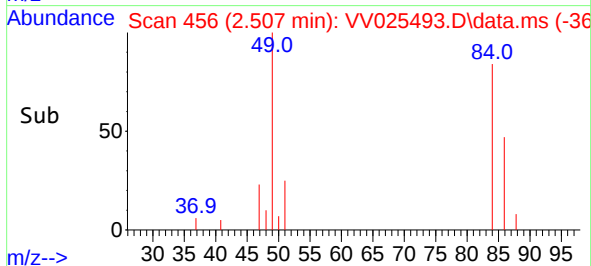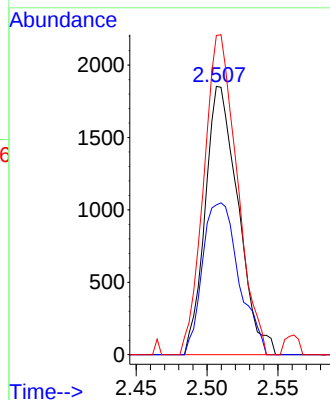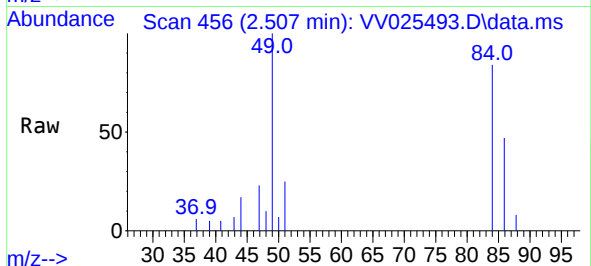

#25
Chloroform
Concen: 0.700 ug/L
RT: 4.378 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VV025493.D
Acq: 13 Apr 2022 15:36

Tgt Ion: 83 Resp: 13707
Ion Ratio Lower Upper
83 100
85 63.9 43.5 80.7

