

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025494.D
 Acq On : 13 Apr 2022 15:59
 Operator : SY/MD
 Sample : N2373-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFD7

Quant Time: Apr 14 03:11:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 03:09:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	133573	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136288	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63498	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	65975	5.313	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.200%
7) Chloroethane-d5	1.571	69	59244	4.484	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.600%
11) 1,1-Dichloroethene-d2	2.111	63	100807	4.052	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.000%
20) 2-Butanone-d5	3.902	46	68868	45.591	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.180%
24) Chloroform-d	4.352	84	93635	4.990	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
26) 1,2-Dichloroethane-d4	5.037	65	43407	5.368	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.400%
32) Benzene-d6	5.053	84	189396	4.803	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
36) 1,2-Dichloropropane-d6	6.069	67	54272	4.935	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.800%
41) Toluene-d8	7.317	98	163528	4.469	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.400%
43) trans-1,3-Dichloroprop...	7.625	79	15273	4.132	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.600%
46) 2-Hexanone-d5	8.088	63	52899	40.776	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.560%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30394	4.375	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	54625	5.131	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds					Qvalue	
25) Chloroform	4.384	83	14312	0.825	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025494.D
Acq On : 13 Apr 2022 15:59
Operator : SY/MD
Sample : N2373-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFD7

Quant Time: Apr 14 03:11:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 03:09:10 2022
Response via : Initial Calibration

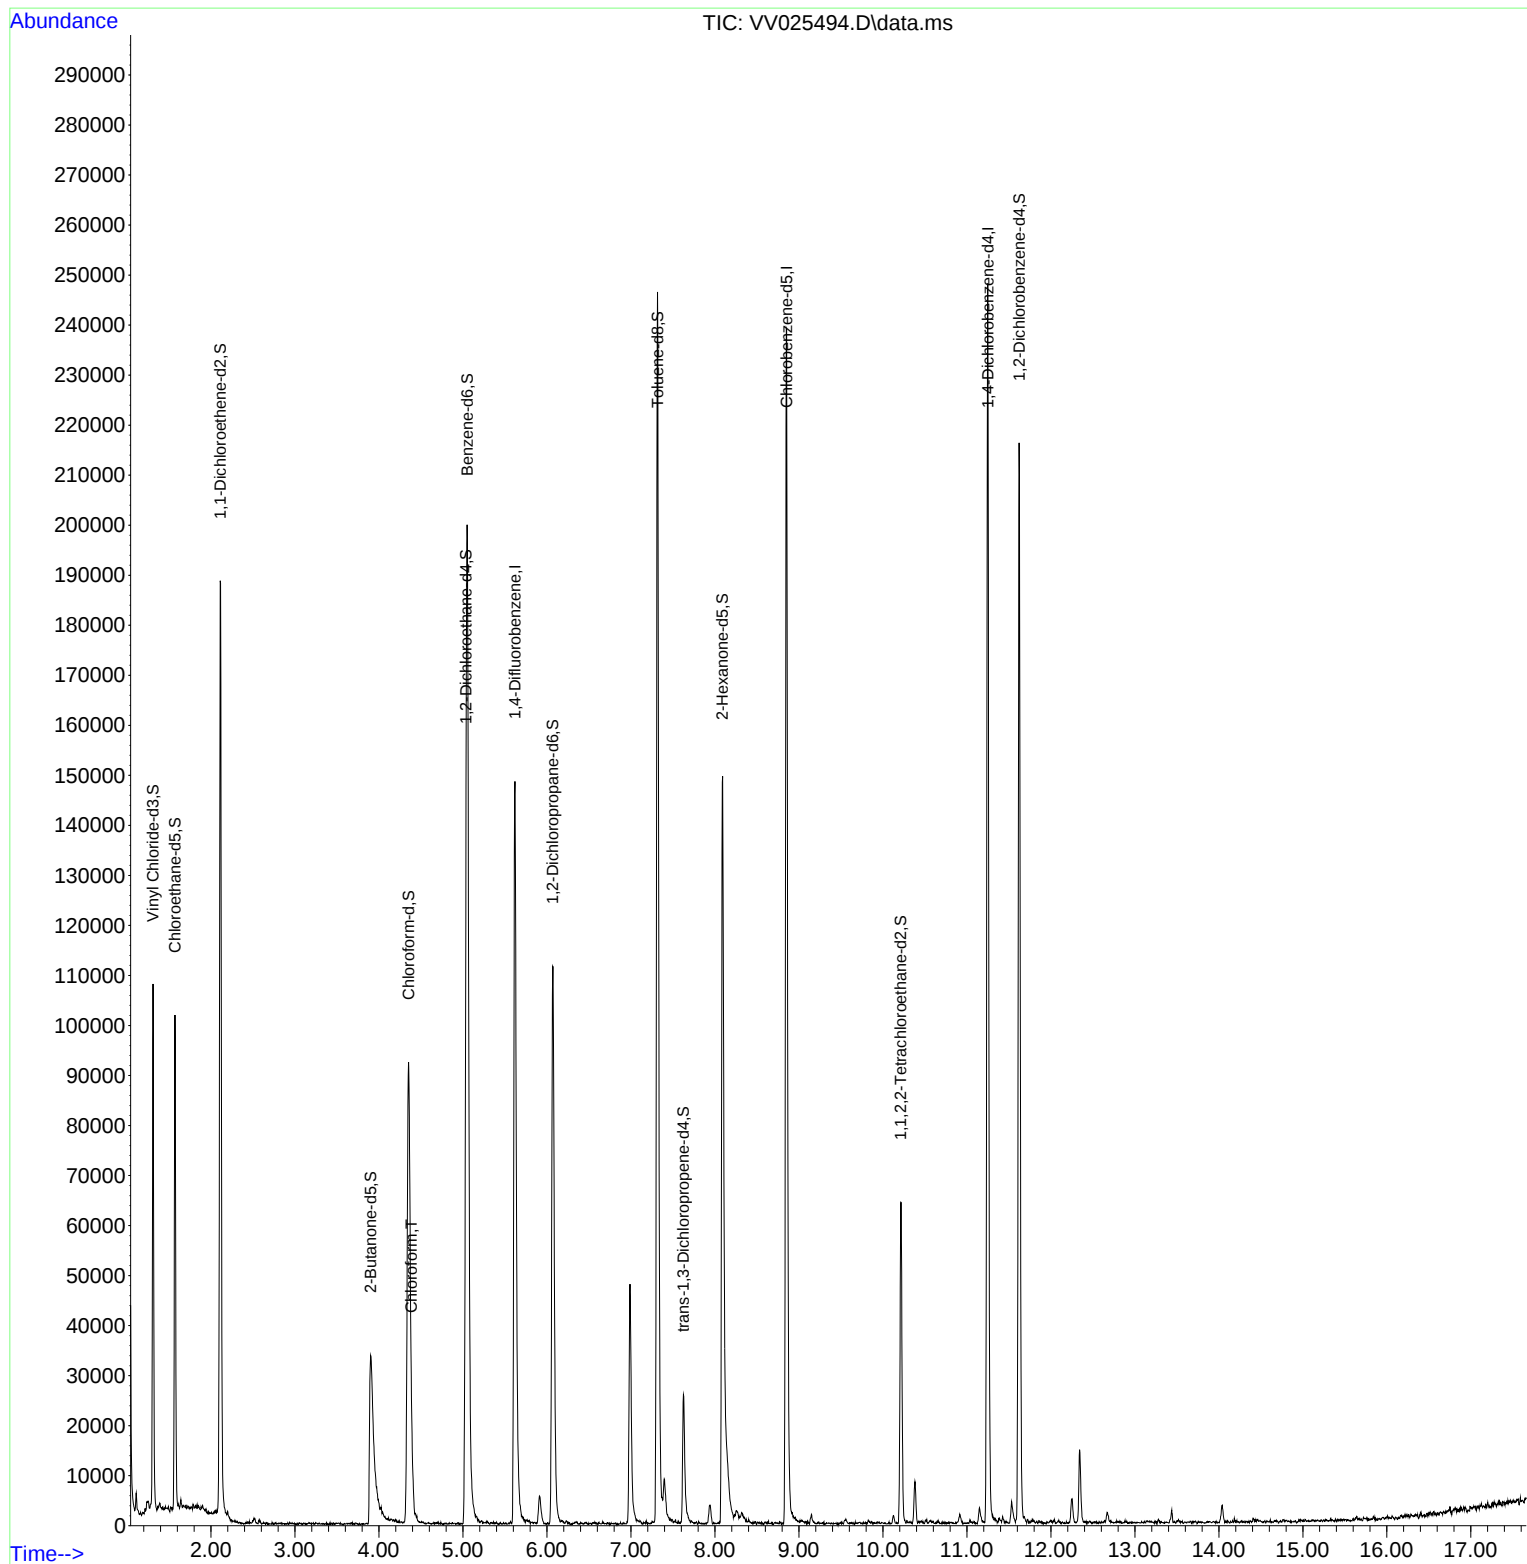

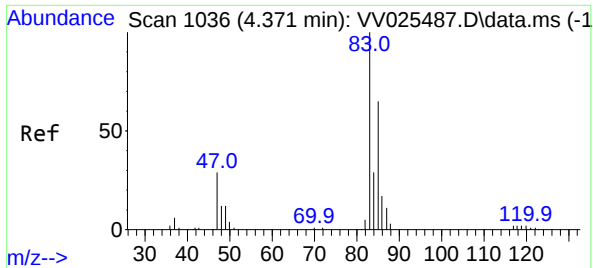

#25
Chloroform
Concen: 0.825 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.013 min
Lab File: VV025494.D
Acq: 13 Apr 2022 15:59

Instrument :
MSVOA_V
ClientSampleId :
BFFD7

Tgt Ion: 83 Resp: 14312
Ion Ratio Lower Upper
83 100
85 66.6 43.5 80.7

