

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025512.D
 Acq On : 13 Apr 2022 23:48
 Operator : SY/MD
 Sample : N2357-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAZ24

Quant Time: Apr 14 05:24:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 05:22:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	95185	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	90863	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	39783	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	49043	5.542	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.800%
7) Chloroethane-d5	1.571	69	48669	5.170	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.400%
11) 1,1-Dichloroethene-d2	2.111	63	69436	3.917	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.400%
20) 2-Butanone-d5	3.905	46	77609	72.097	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	144.200%#
24) Chloroform-d	4.355	84	80014	5.983	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	119.600%
26) 1,2-Dichloroethane-d4	5.037	65	39363	6.832	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	136.600%#
32) Benzene-d6	5.053	84	150318	5.718	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.400%
36) 1,2-Dichloropropane-d6	6.069	67	46624	6.359	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	127.200%
41) Toluene-d8	7.317	98	112019	4.591	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.800%
43) trans-1,3-Dichloroprop...	7.628	79	10657	4.324	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.400%
46) 2-Hexanone-d5	8.091	63	54999	63.588	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	127.180%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31996	6.907	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	138.200%#
66) 1,2-Dichlorobenzene-d4	11.622	152	39309	5.893	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.800%
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.301	76	1626	0.082	ug/L #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025512.D
Acq On : 13 Apr 2022 23:48
Operator : SY/MD
Sample : N2357-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ24

Quant Time: Apr 14 05:24:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 05:22:13 2022
Response via : Initial Calibration

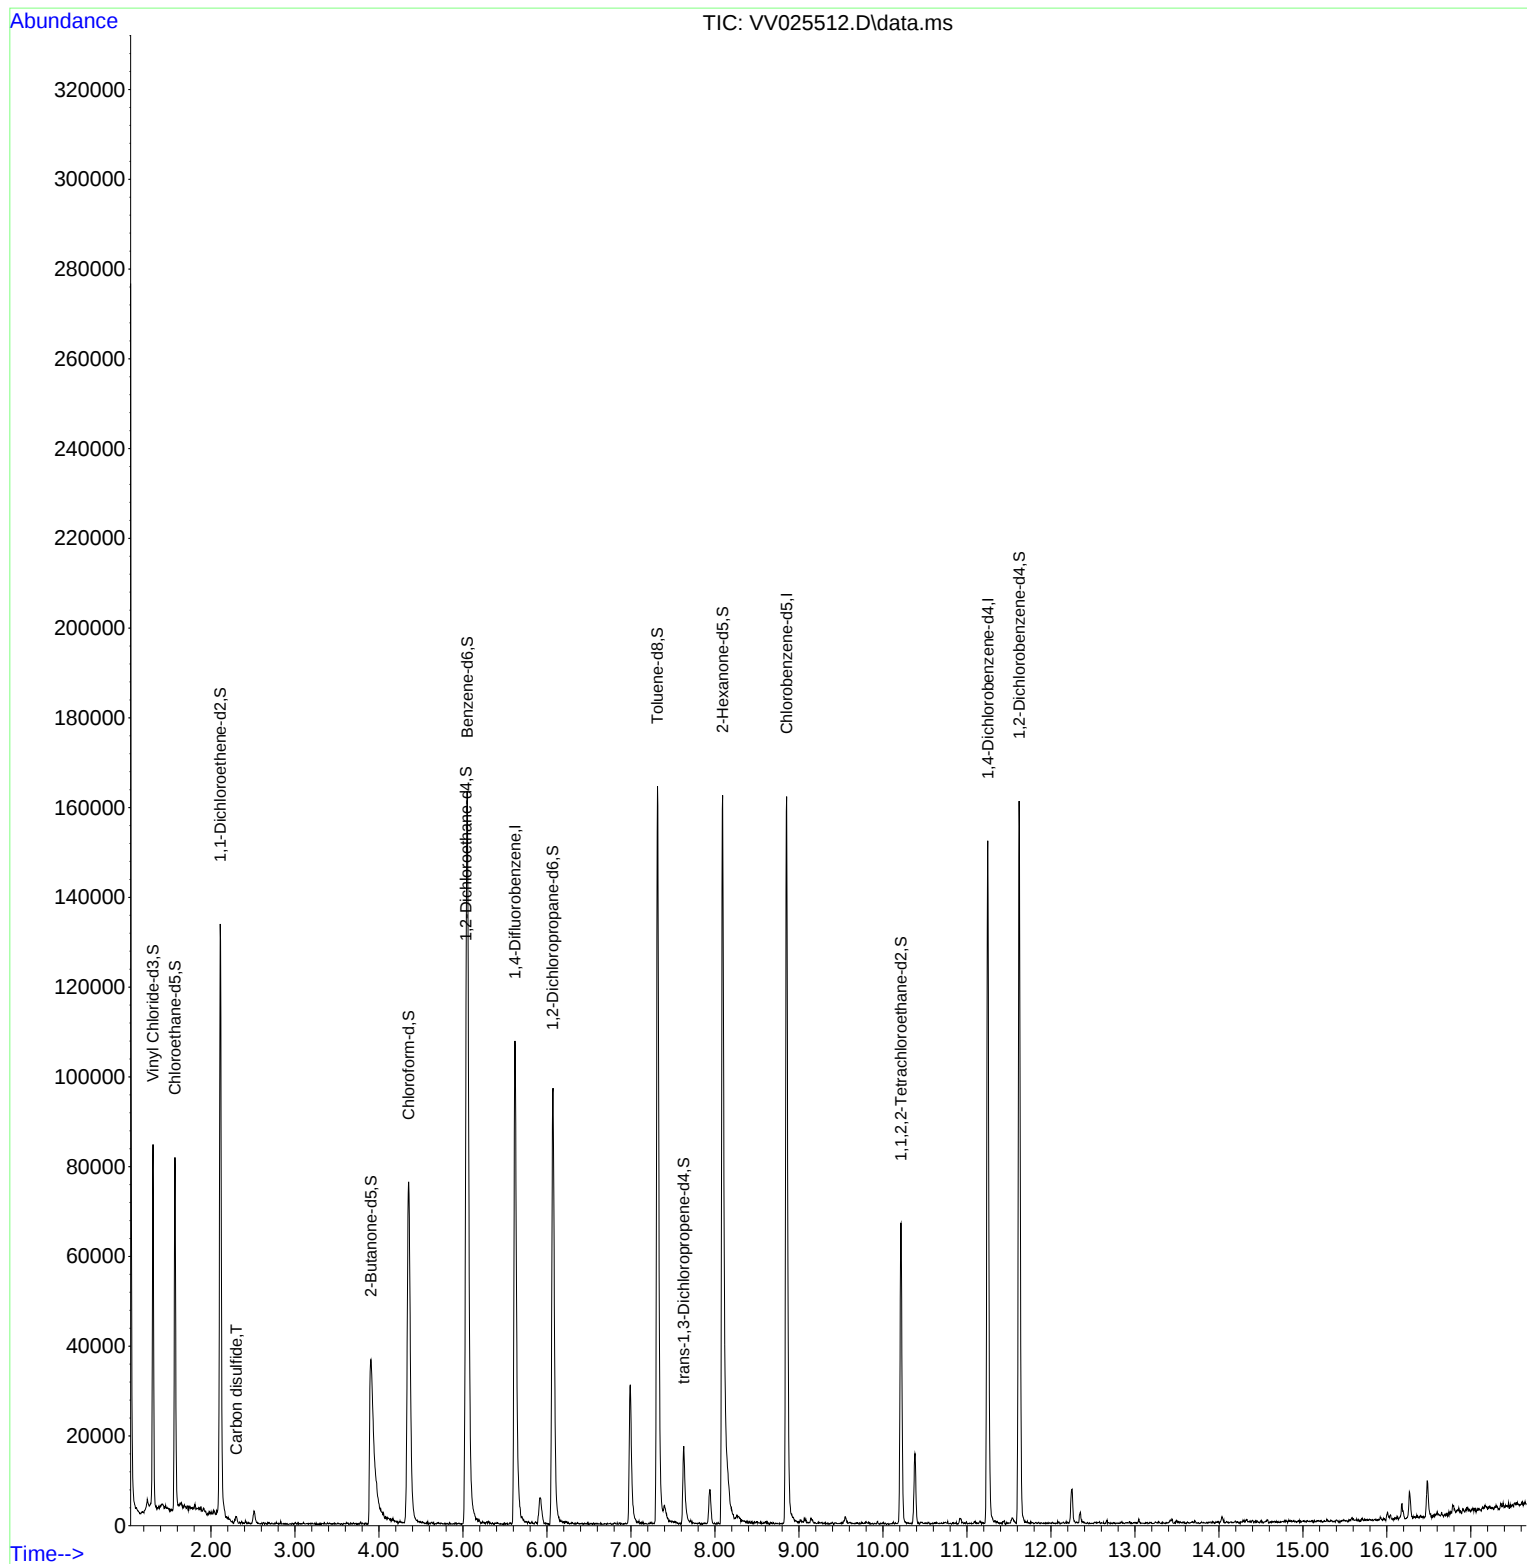

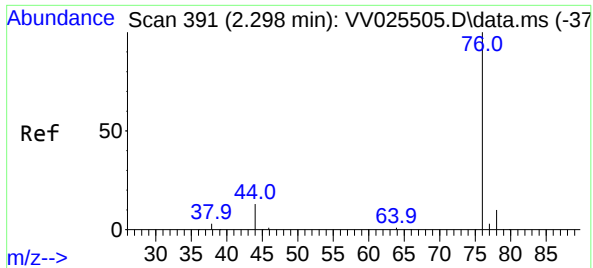

#14
Carbon disulfide
Concen: 0.082 ug/L
RT: 2.301 min Scan# 391
Delta R.T. 0.003 min
Lab File: VV025512.D
Acq: 13 Apr 2022 23:48

Instrument :
MSVOA_V
ClientSampleId :
YAZ24

Tgt Ion: 76 Resp: 1626
Ion Ratio Lower Upper
76 100
78 17.5 7.3 10.9#

