

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025514.D
 Acq On : 14 Apr 2022 00:34
 Operator : SY/MD
 Sample : N2388-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE5

Quant Time: Apr 14 05:24:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 05:22:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	129019	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	130422	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58961	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	64512	5.378	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	107.600%	
7) Chloroethane-d5	1.571	69	57891	4.537	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.800%	
11) 1,1-Dichloroethene-d2	2.111	63	97935	4.076	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	81.600%	
20) 2-Butanone-d5	3.902	46	69387	47.555	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	95.120%	
24) Chloroform-d	4.352	84	89102	4.916	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	5.037	65	41067	5.258	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.200%	
32) Benzene-d6	5.053	84	180613	4.786	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.069	67	52842	5.021	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.400%	
41) Toluene-d8	7.317	98	152998	4.369	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.400%	
43) trans-1,3-Dichloroprop...	7.625	79	13767	3.892	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	77.800%	
46) 2-Hexanone-d5	8.092	63	49329	39.734	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	79.460%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	28525	4.290	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	85.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50389	5.097	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.000%	
Target Compounds					Qvalue	
25) Chloroform	4.378	83	13755	0.820	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025514.D
Acq On : 14 Apr 2022 00:34
Operator : SY/MD
Sample : N2388-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFE5

Quant Time: Apr 14 05:24:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 05:22:13 2022
Response via : Initial Calibration

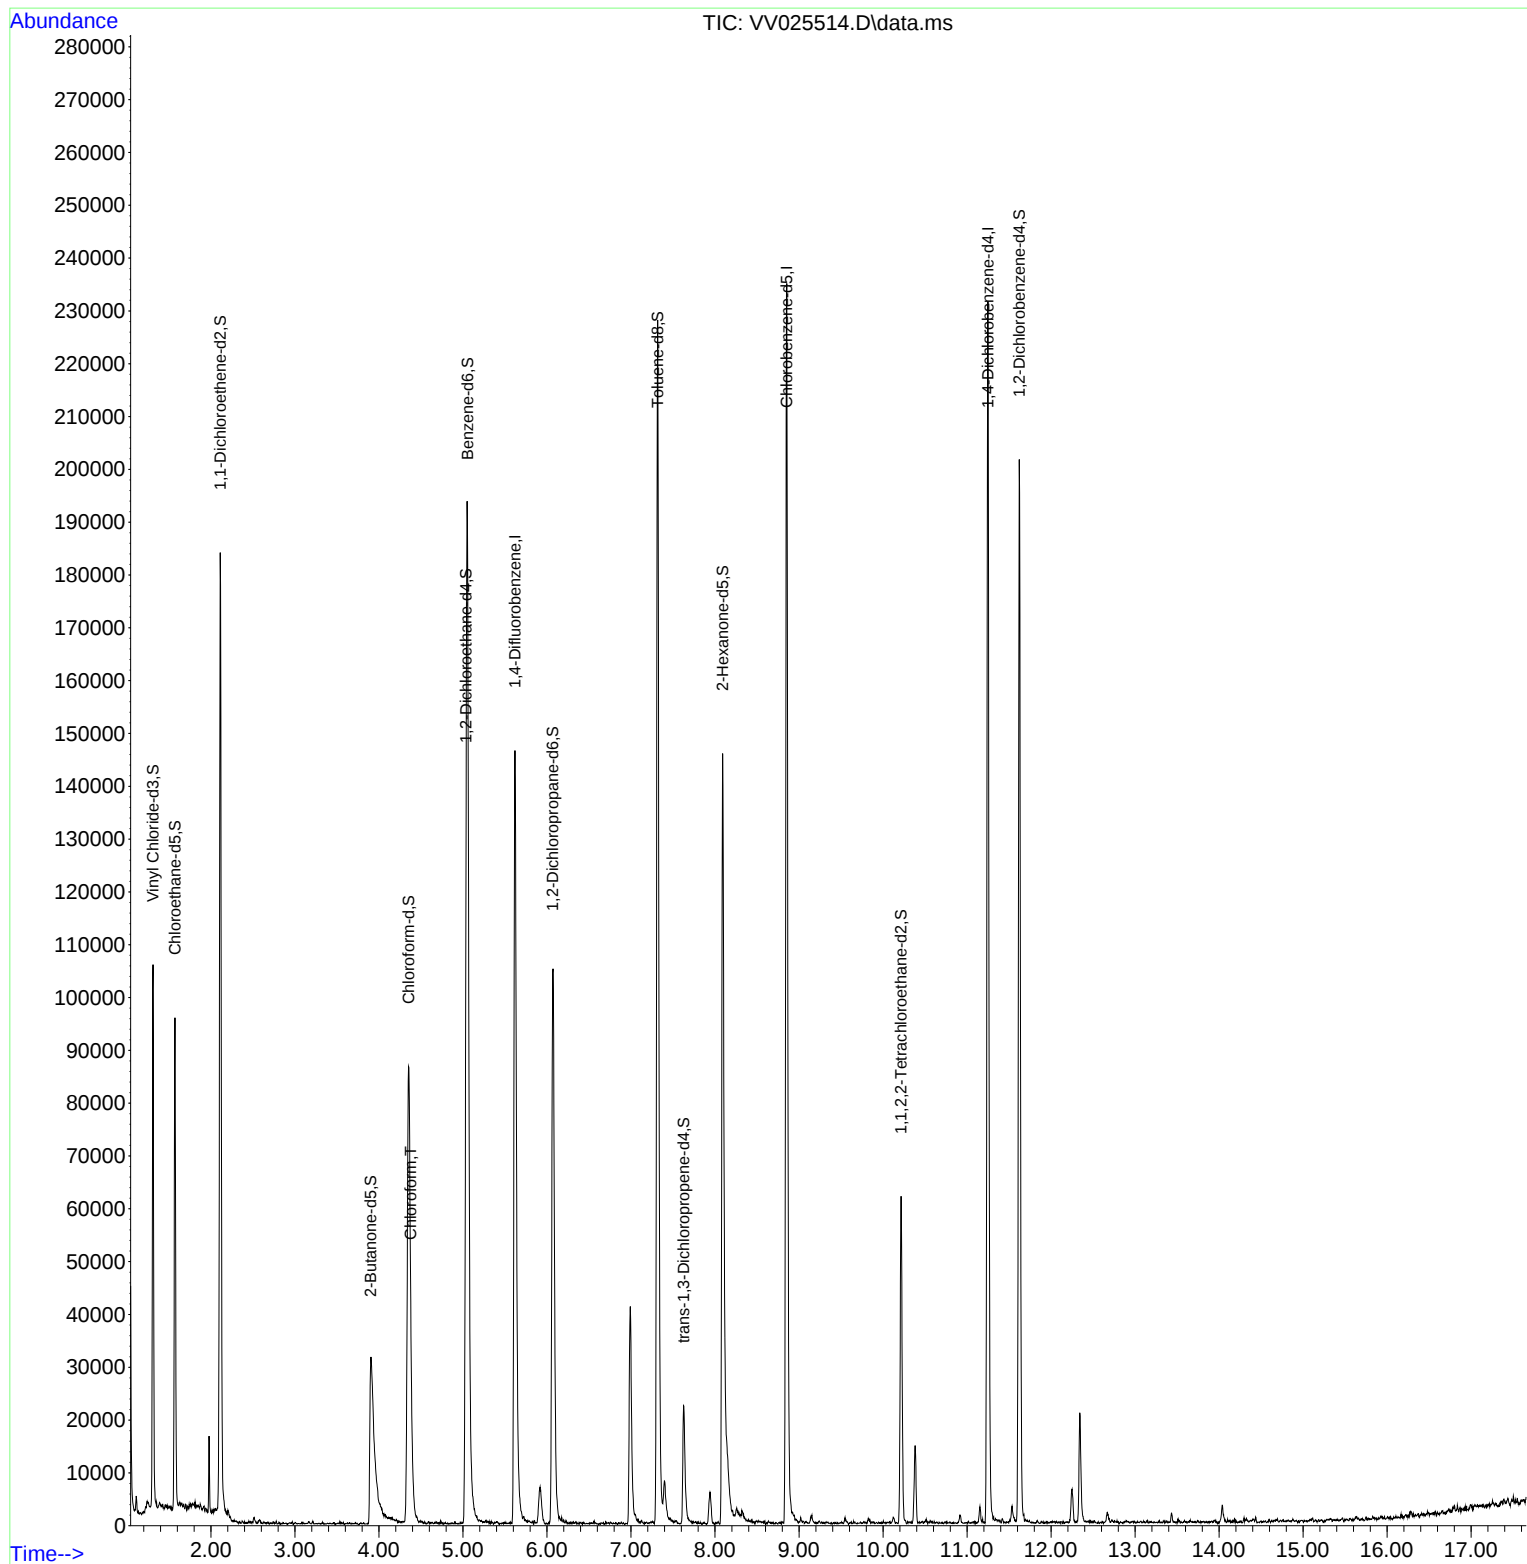

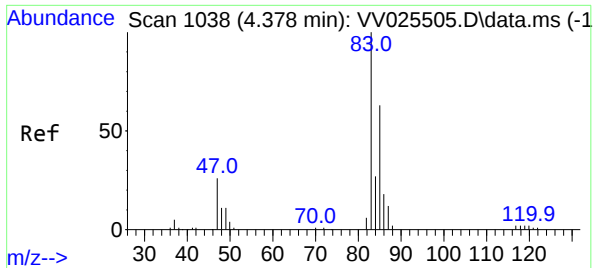

#25
 Chloroform
 Concen: 0.820 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: VV025514.D
 Acq: 14 Apr 2022 00:34

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE5

Tgt Ion: 83 Resp: 13755
 Ion Ratio Lower Upper
 83 100
 85 62.5 43.5 80.7

