

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025515.D
 Acq On : 14 Apr 2022 00:58
 Operator : SY/MD
 Sample : N2388-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE6

Quant Time: Apr 14 05:24:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 05:22:13 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123682	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	124983	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56352	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	62562	5.441	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 108.800%		
7) Chloroethane-d5	1.571	69	55874	4.567	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 91.400%		
11) 1,1-Dichloroethene-d2	2.111	63	92753	4.027	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 80.600%		
20) 2-Butanone-d5	3.902	46	66388	47.463	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 94.920%		
24) Chloroform-d	4.352	84	84690	4.874	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 97.400%		
26) 1,2-Dichloroethane-d4	5.037	65	40144	5.362	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 107.200%		
32) Benzene-d6	5.053	84	173499	4.798	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 96.000%		
36) 1,2-Dichloropropane-d6	6.069	67	50407	4.998	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 100.000%		
41) Toluene-d8	7.316	98	147511	4.396	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 88.000%		
43) trans-1,3-Dichloroprop...	7.628	79	13151	3.880	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 77.600%		
46) 2-Hexanone-d5	8.091	63	47068	39.563	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 79.120%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	28469	4.468	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 89.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	47864	5.066	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 101.400%		
Target Compounds						
13) Acetone	2.191	43	3898	4.106	ug/L	86
25) Chloroform	4.384	83	14933	0.929	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025515.D
Acq On : 14 Apr 2022 00:58
Operator : SY/MD
Sample : N2388-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFE6

Quant Time: Apr 14 05:24:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 05:22:13 2022
Response via : Initial Calibration




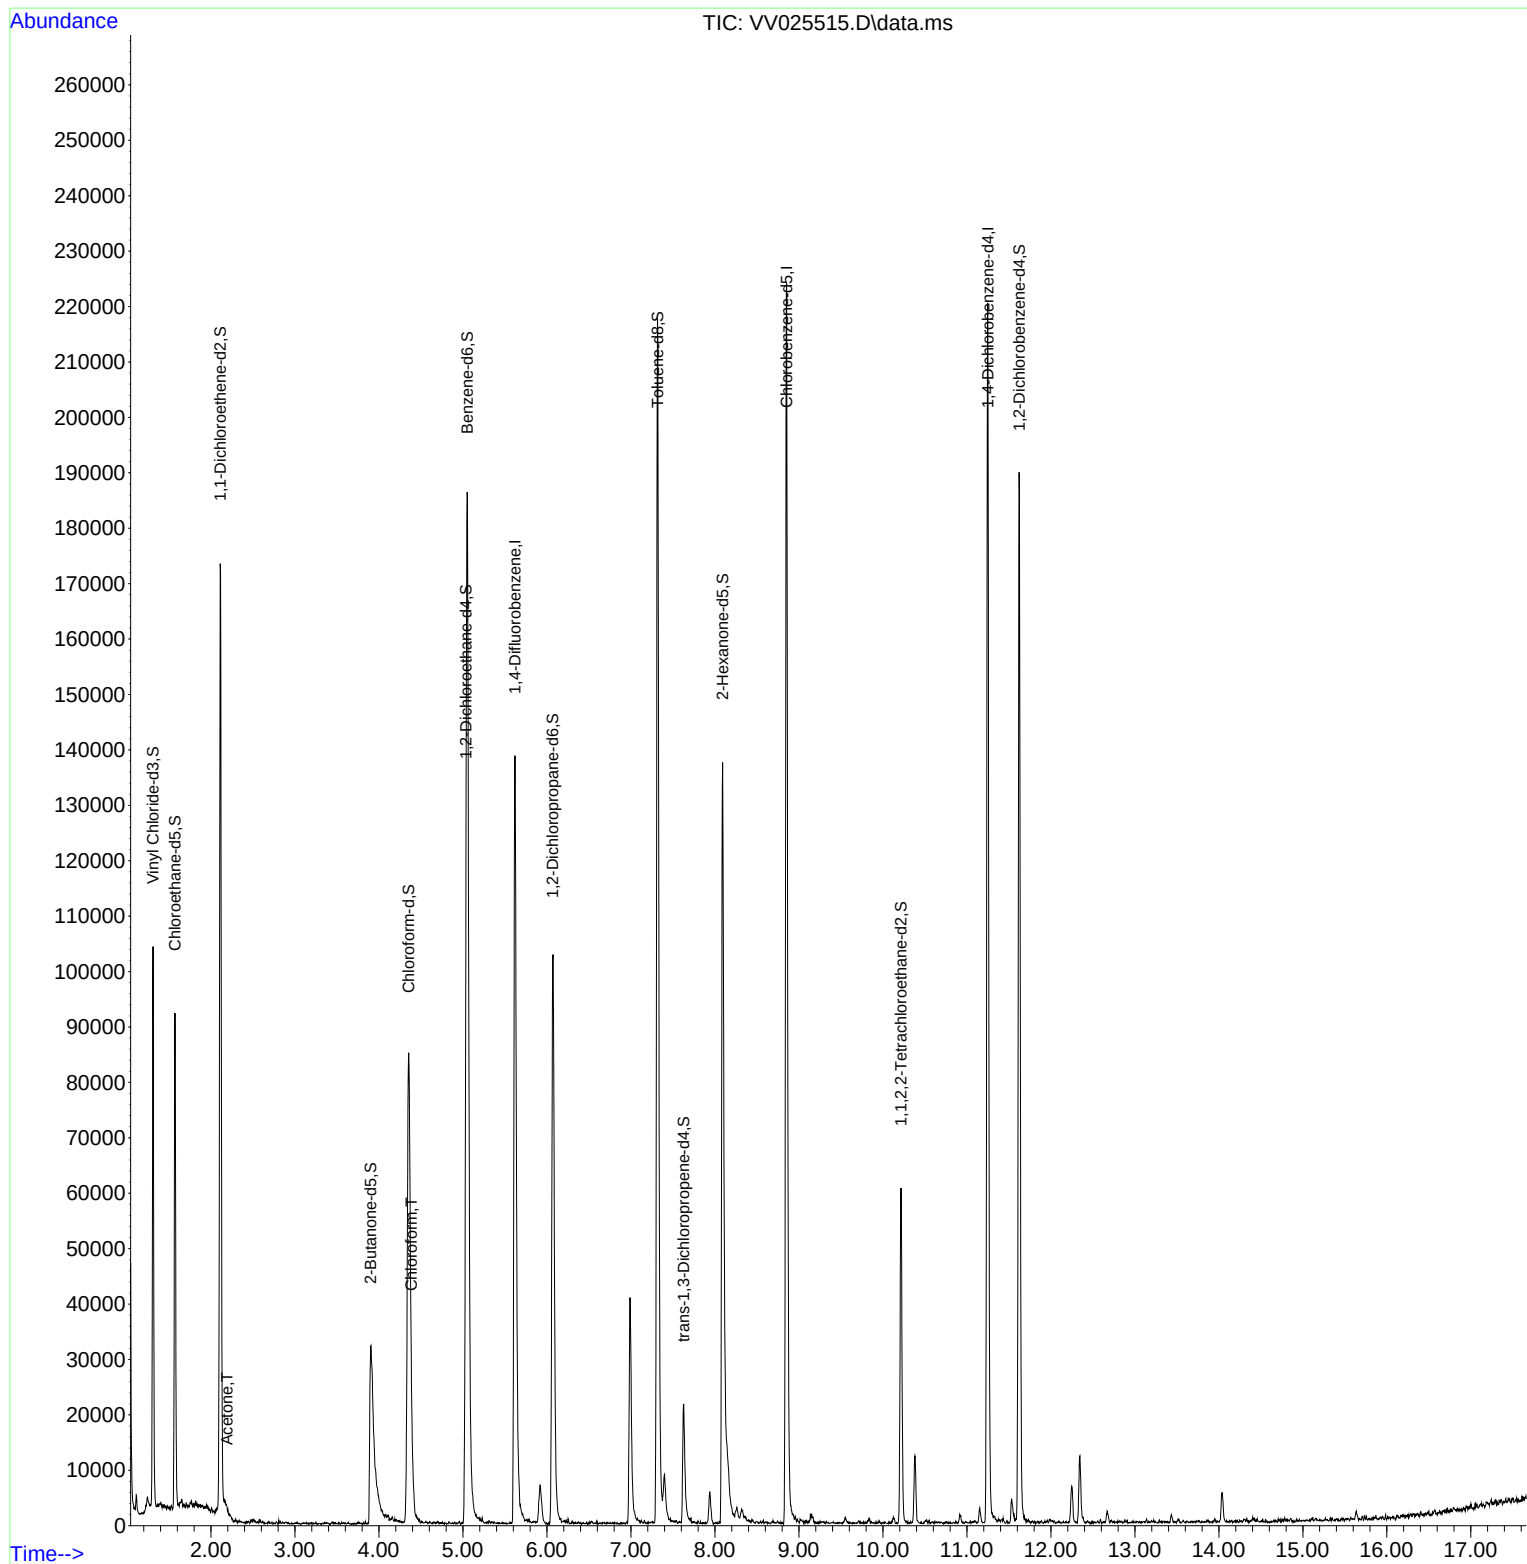


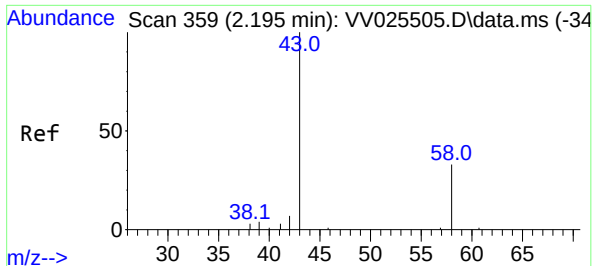

#13
Acetone
Concen: 4.106 ug/L
RT: 2.191 min Scan# 31
Delta R.T. -0.003 min
Lab File: VV025515.D
Acq: 14 Apr 2022 00:58

Instrument :
MSVOA_V
ClientSampleId :
BFFE6

Tgt Ion: 43 Resp: 3898
Ion Ratio Lower Upper
43 100
58 27.7 0.0 72.2

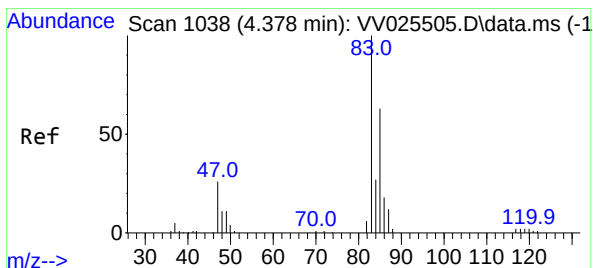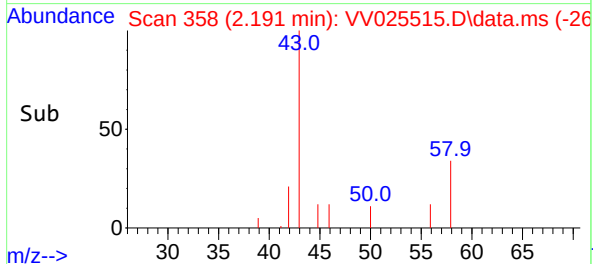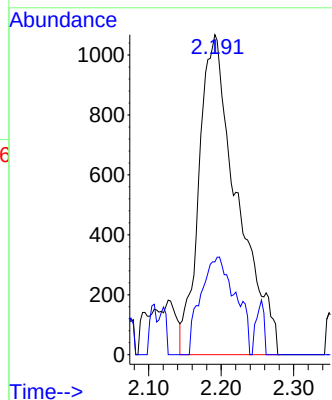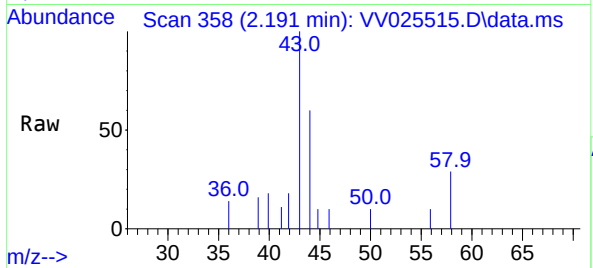

#25
Chloroform
Concen: 0.929 ug/L
RT: 4.384 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VV025515.D
Acq: 14 Apr 2022 00:58

Tgt Ion: 83 Resp: 14933
Ion Ratio Lower Upper
83 100
85 62.5 43.5 80.7

