

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025518.D
 Acq On : 14 Apr 2022 02:08
 Operator : SY/MD
 Sample : N2384-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R4

Quant Time: Apr 14 05:25:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 05:22:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	128754	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	127773	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59806	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	67488	5.638	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	112.800%	
7) Chloroethane-d5	1.571	69	58441	4.589	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.111	63	99677	4.157	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	83.200%	
20) 2-Butanone-d5	3.934	46	53626	36.829	ug/L	0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	73.660%	
24) Chloroform-d	4.352	84	87165	4.819	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4	5.037	65	39380	5.053	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.000%	
32) Benzene-d6	5.053	84	173188	4.685	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.600%	
36) 1,2-Dichloropropane-d6	6.072	67	49577	4.809	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.200%	
41) Toluene-d8	7.316	98	144510	4.212	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.200%	
43) trans-1,3-Dichloroprop...	7.625	79	14350	4.141	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.800%	
46) 2-Hexanone-d5	8.091	63	49315	40.546	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	81.100%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29283	4.496	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	48964	4.883	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.600%	
Target Compounds						
					Qvalue	
16) Methylene chloride	2.513	84	4191	0.387	ug/L	94
25) Chloroform	4.378	83	12799	0.765	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025518.D
Acq On : 14 Apr 2022 02:08
Operator : SY/MD
Sample : N2384-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6R4

Quant Time: Apr 14 05:25:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 05:22:13 2022
Response via : Initial Calibration




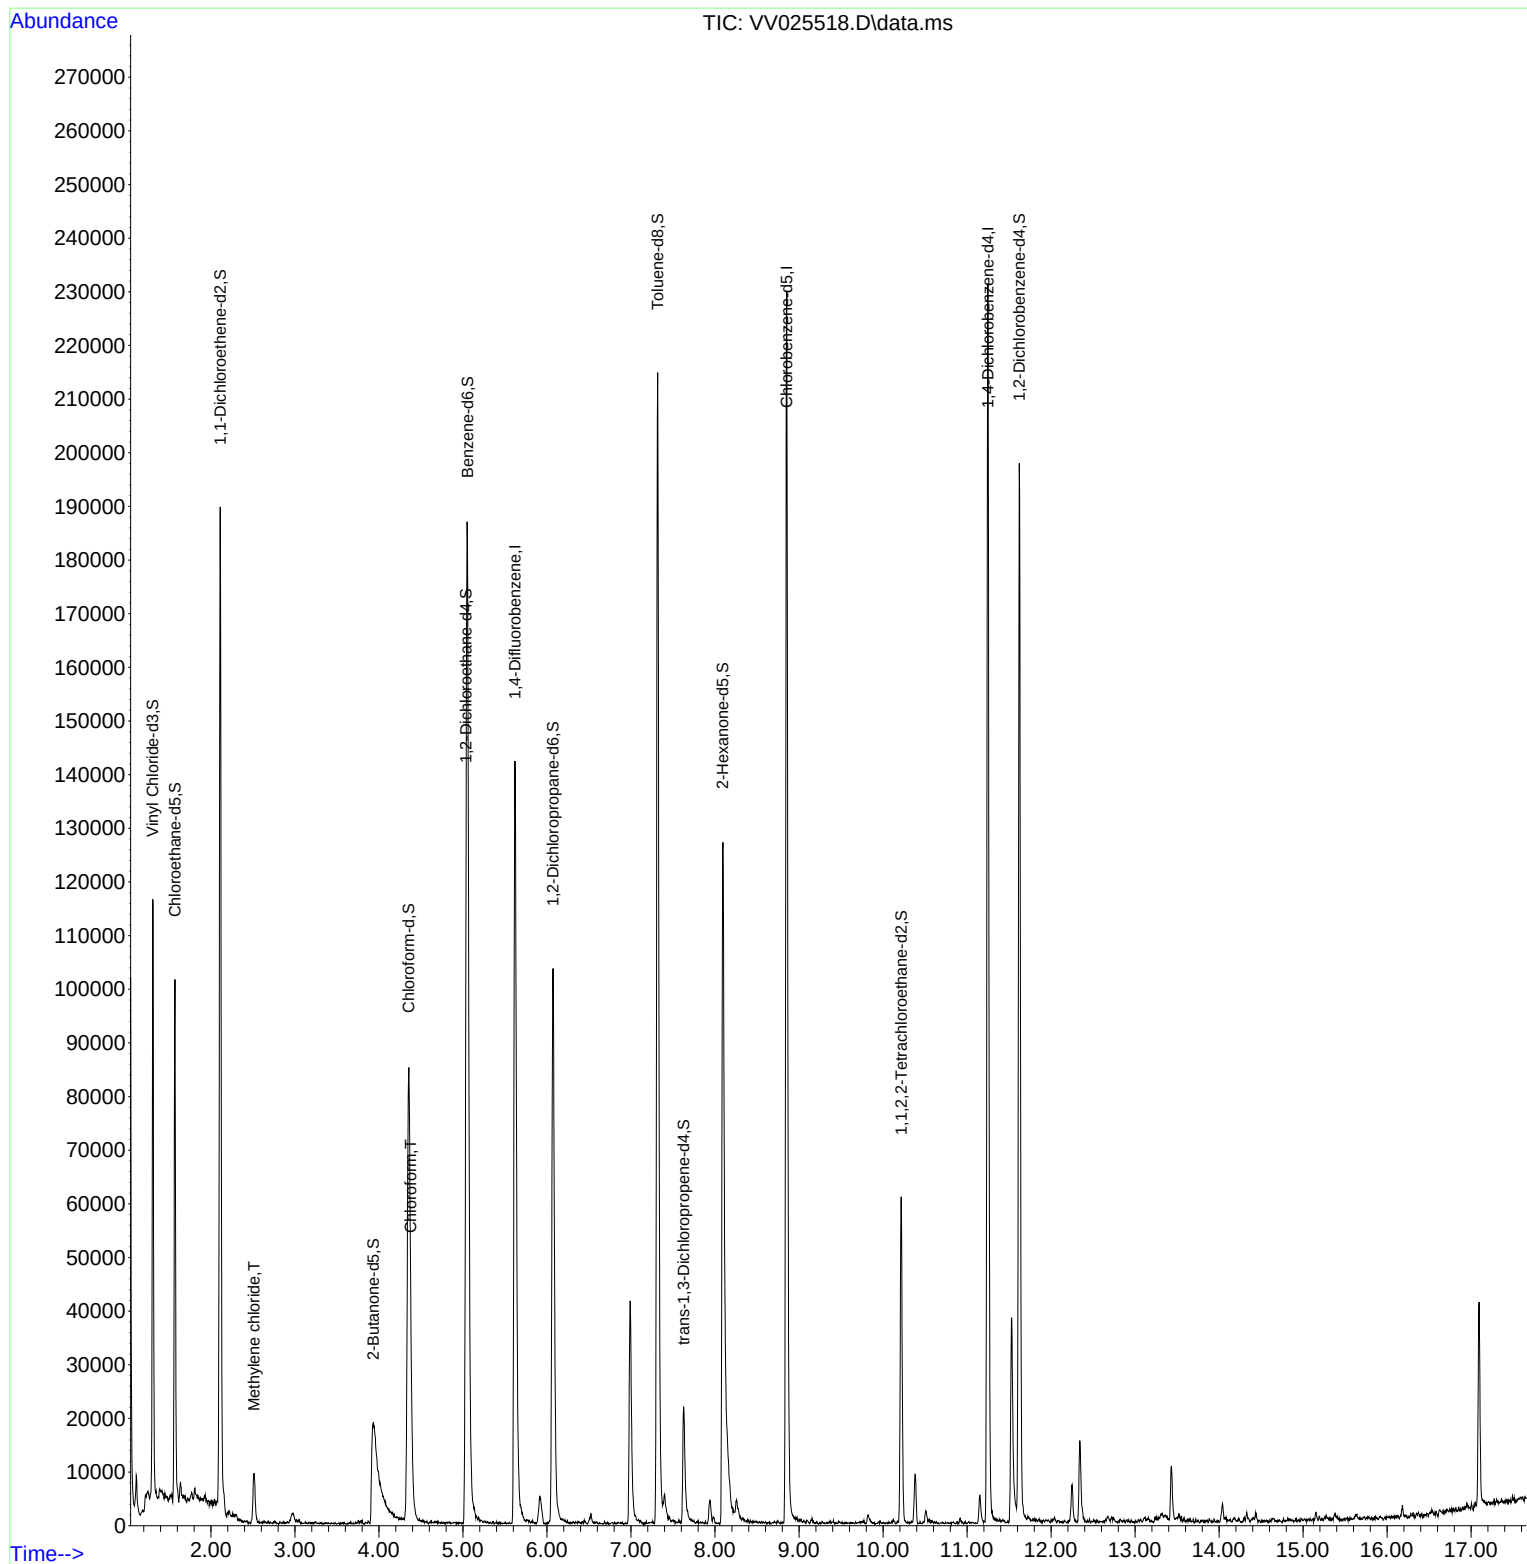


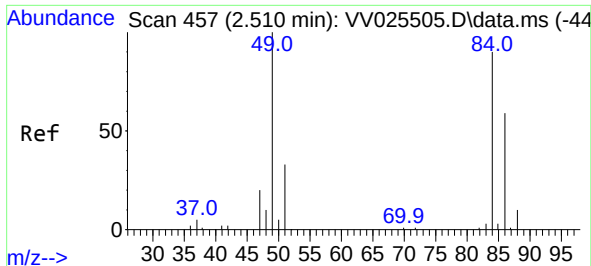

#16
Methylene chloride
Concen: 0.387 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV025518.D
Acq: 14 Apr 2022 02:08

Instrument :
MSVOA_V
ClientSampleId :
EW6R4

Tgt Ion: 84 Resp: 4191
Ion Ratio Lower Upper
84 100
86 58.1 45.9 85.3
49 105.3 76.6 142.3

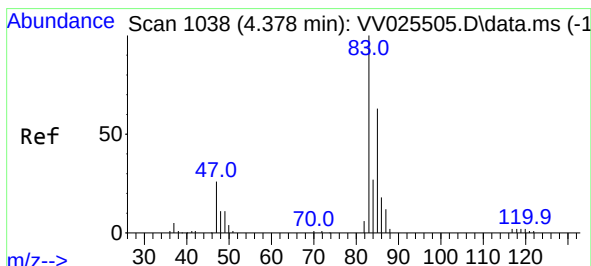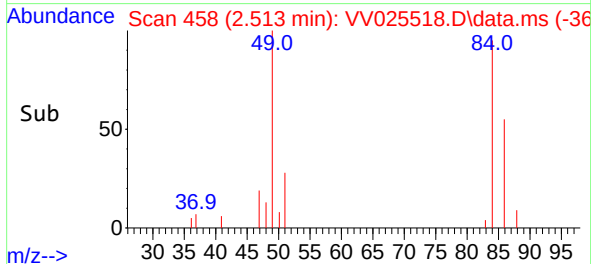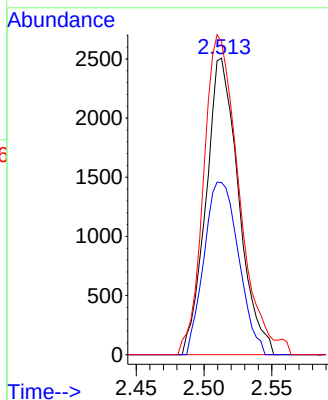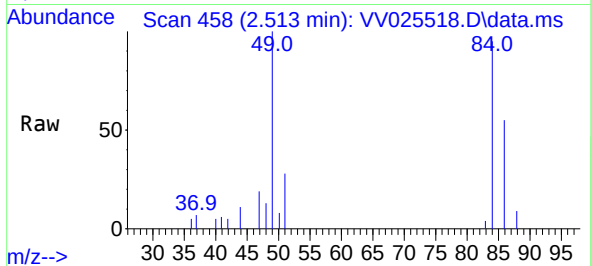

#25
Chloroform
Concen: 0.765 ug/L
RT: 4.378 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VV025518.D
Acq: 14 Apr 2022 02:08

Tgt Ion: 83 Resp: 12799
Ion Ratio Lower Upper
83 100
85 67.3 43.5 80.7

