

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041322\
 Data File : VW025522.D
 Acq On : 14 Apr 2022 03:41
 Operator : SY/MD
 Sample : N2384-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6P6

Quant Time: Apr 14 05:25:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 14 05:22:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121018	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	121788	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54688	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	61739	5.487	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.800%
7) Chloroethane-d5	1.571	69	55368	4.626	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.600%
11) 1,1-Dichloroethene-d2	2.111	63	95236	4.225	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.600%
20) 2-Butanone-d5	3.924	46	59994	43.836	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.680%
24) Chloroform-d	4.355	84	85914	5.053	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.000%
26) 1,2-Dichloroethane-d4	5.037	65	40074	5.470	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.400%
32) Benzene-d6	5.053	84	170401	4.836	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	6.072	67	49296	5.016	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.317	98	142546	4.359	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.628	79	13292	4.024	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.091	63	51226	44.187	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.380%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30761	4.955	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	47829	5.216	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.400%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.134	85	720	0.066	ug/L	95
53) m,p-Xylene	9.146	106	1251	0.079	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025522.D
Acq On : 14 Apr 2022 03:41
Operator : SY/MD
Sample : N2384-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6P6

Quant Time: Apr 14 05:25:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 14 05:22:13 2022
Response via : Initial Calibration




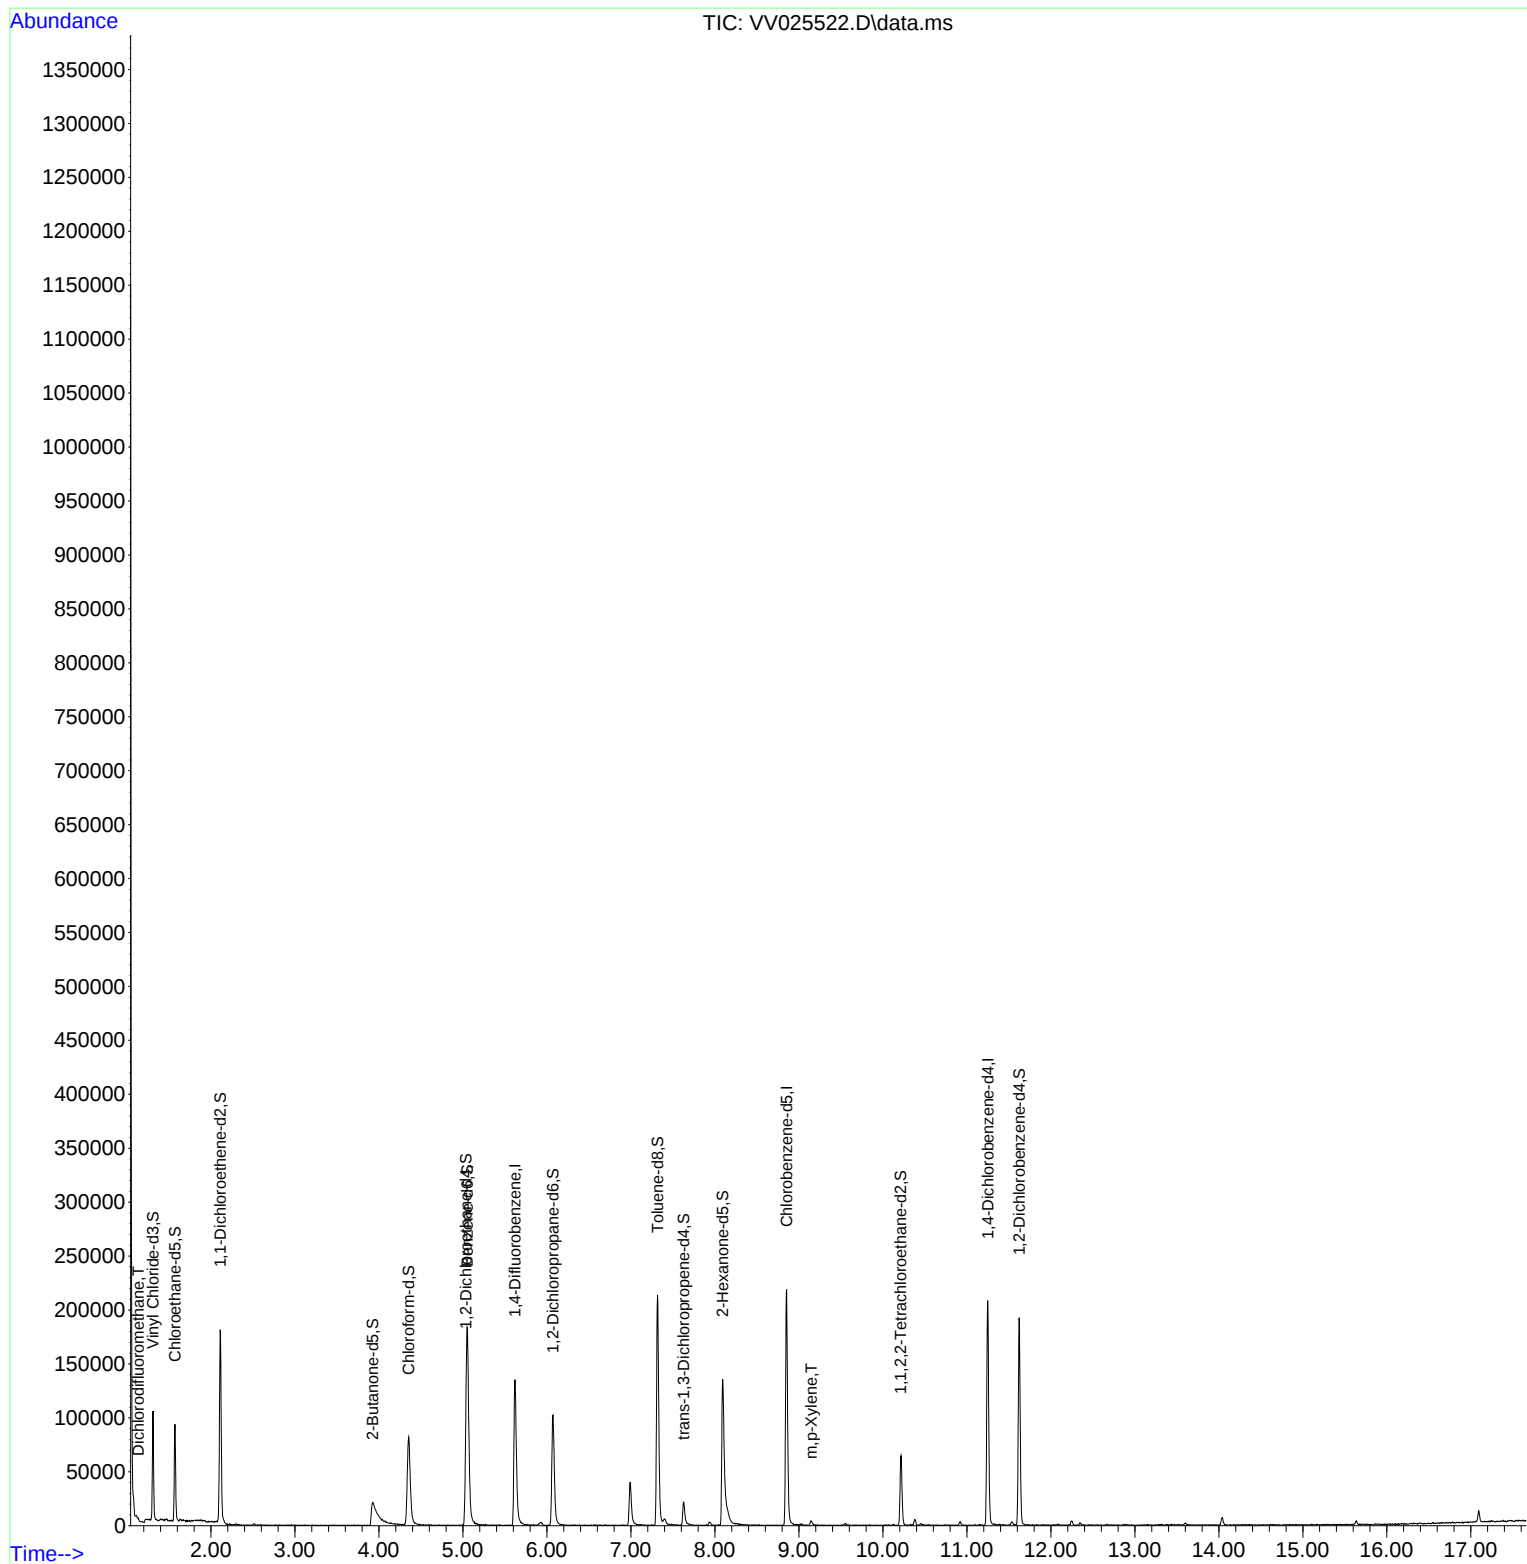


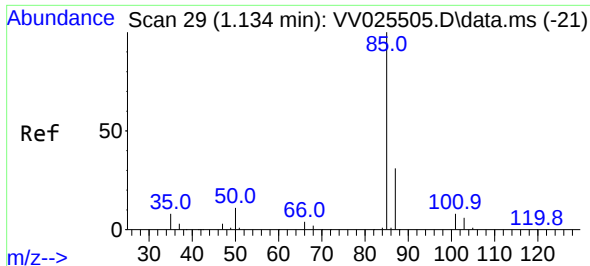

#2
Dichlorodifluoromethane
Concen: 0.066 ug/L
RT: 1.134 min Scan# 29
Delta R.T. -0.000 min
Lab File: VV025522.D
Acq: 14 Apr 2022 03:41

Instrument :
MSVOA_V
ClientSampleId :
EW6P6

Tgt Ion: 85 Resp: 720
Ion Ratio Lower Upper
85 100
87 34.7 25.6 38.4

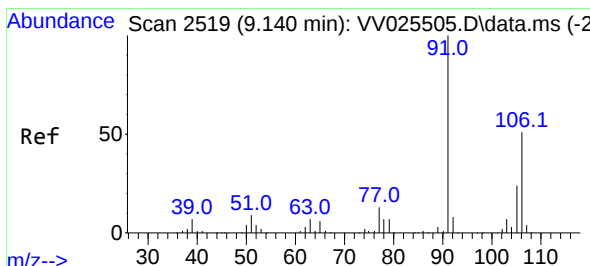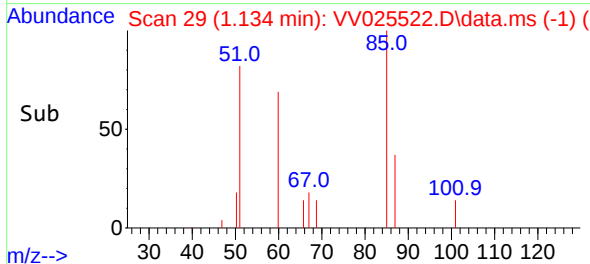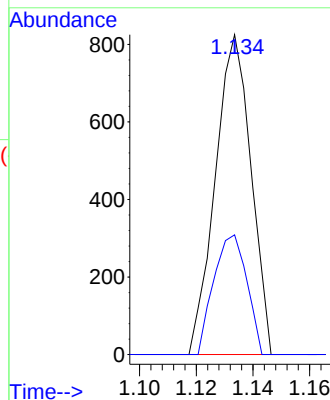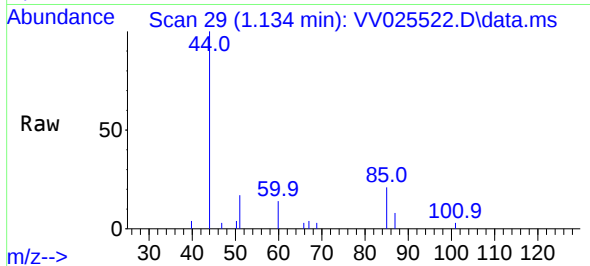

#53
m,p-Xylene
Concen: 0.079 ug/L
RT: 9.146 min Scan# 2521
Delta R.T. 0.006 min
Lab File: VV025522.D
Acq: 14 Apr 2022 03:41

Tgt Ion: 106 Resp: 1251
Ion Ratio Lower Upper
106 100
91 223.2 136.4 253.4

