

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
 Data File : VV025490.D
 Acq On : 13 Apr 2022 13:15
 Operator : SY/MD
 Sample : N2372-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	95	rVB	106492	108162	22.87%	2.769%
2	1.574	157	166	175	rBV	90857	103272	21.84%	2.644%
3	2.111	322	333	352	rVB	185752	273268	57.79%	6.995%
4	2.516	446	459	467	rBV5	3434	5974	1.26%	0.153%
5	3.908	883	892	925	rBV	26322	104518	22.10%	2.675%
6	4.352	1015	1030	1056	rBV2	81515	210465	44.51%	5.387%
7	5.050	1232	1247	1268	rBV2	191774	472851	100.00%	12.104%
8	5.619	1411	1424	1447	rBV	157867	320987	67.88%	8.217%
9	5.915	1507	1516	1529	rBV10	3996	8475	1.79%	0.217%
10	6.072	1551	1565	1586	rBV	102368	216421	45.77%	5.540%
11	6.989	1840	1850	1868	rBV	43998	82923	17.54%	2.123%
12	7.317	1940	1952	1973	rBV	230992	408710	86.44%	10.462%
13	7.397	1974	1977	1991	rVB7	3612	6044	1.28%	0.155%
14	7.625	2038	2048	2063	rBV	23391	43482	9.20%	1.113%
15	8.091	2183	2193	2228	rBV	136601	290389	61.41%	7.433%
16	8.853	2418	2430	2448	rBV	248689	411436	87.01%	10.532%
17	10.217	2843	2854	2871	rBV	61920	97785	20.68%	2.503%
18	11.249	3162	3175	3195	rBV	260140	409997	86.71%	10.495%
19	11.622	3280	3291	3309	rBV	196190	316987	67.04%	8.114%
20	12.249	3476	3486	3495	rBV	4152	6832	1.44%	0.175%
21	14.043	4031	4044	4051	rBV2	4386	7572	1.60%	0.194%




Sum of corrected areas: 3906550

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025490.D
Acq On : 13 Apr 2022 13:15
Operator : SY/MD
Sample : N2372-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

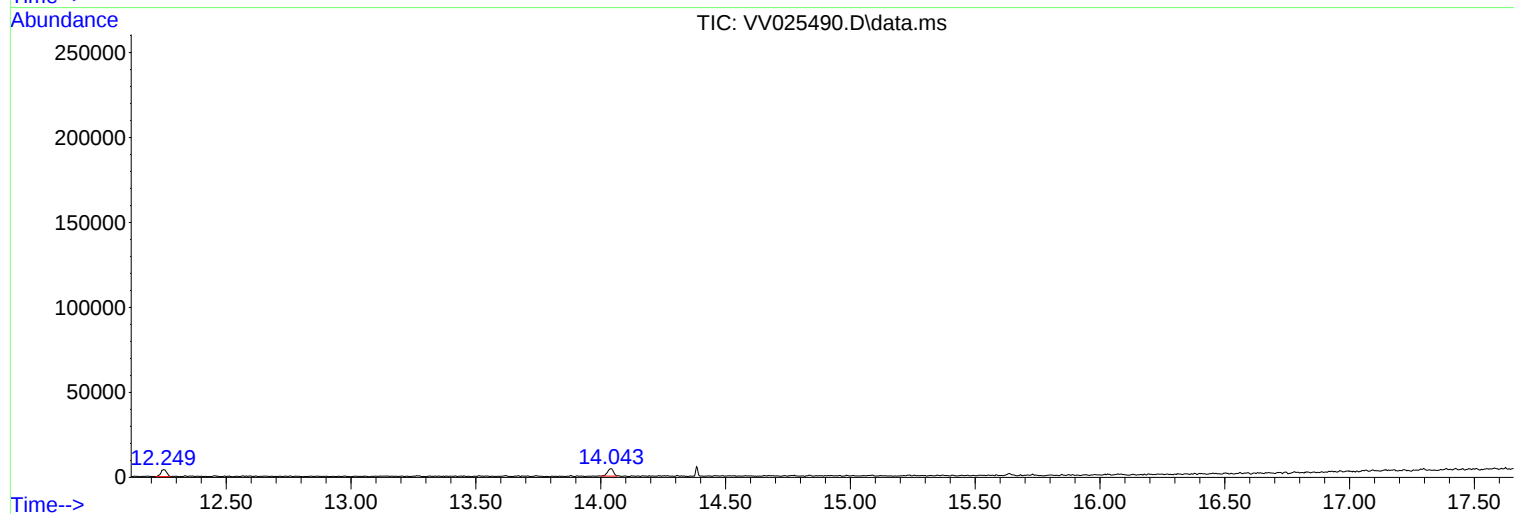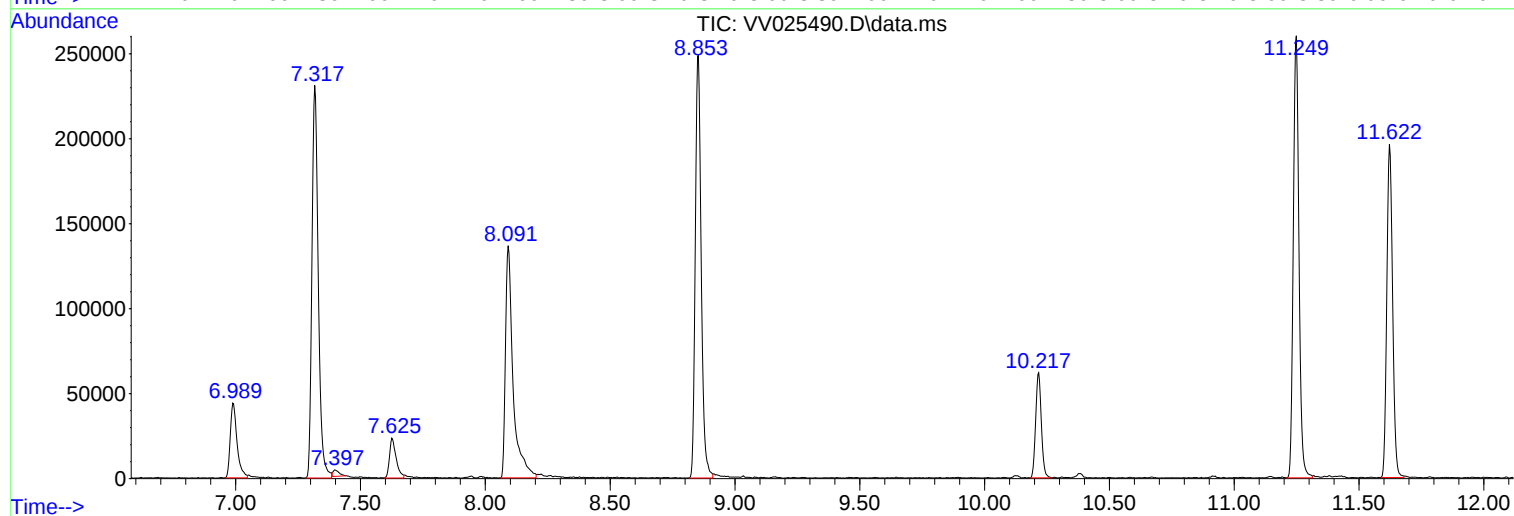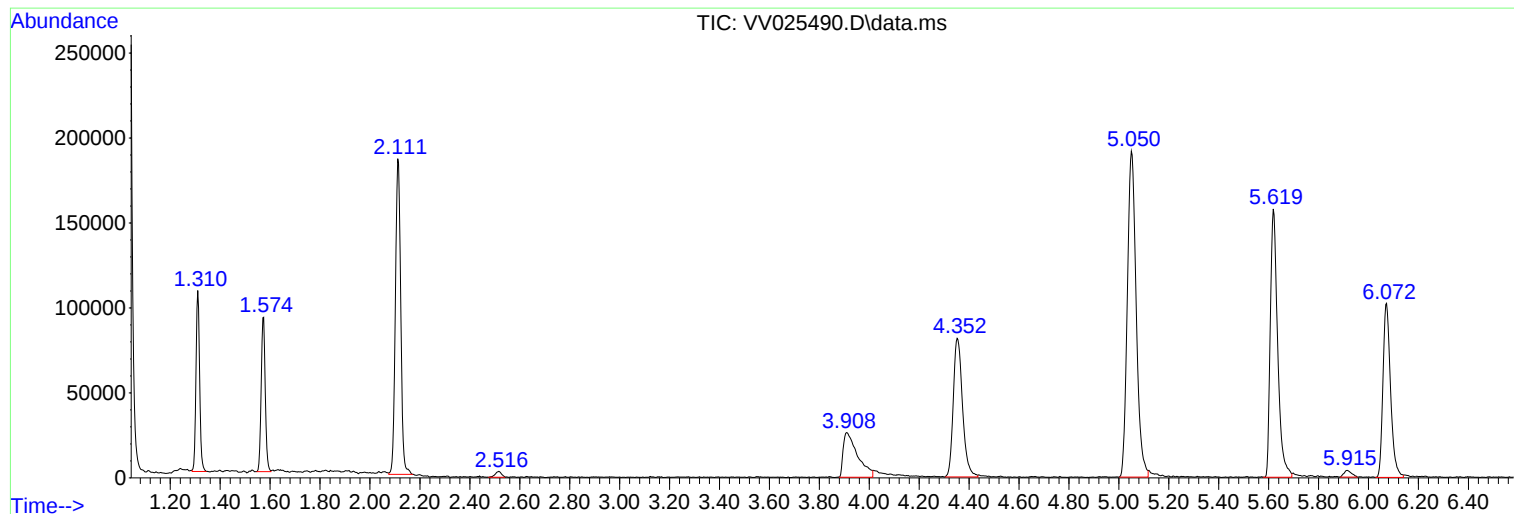

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025490.D
Acq On : 13 Apr 2022 13:15
Operator : SY/MD
Sample : N2372-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025490.D
Acq On : 13 Apr 2022 13:15
Operator : SY/MD
Sample : N2372-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
