

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
 Data File : VV025491.D
 Acq On : 13 Apr 2022 13:39
 Operator : SY/MD
 Sample : N2319-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	97	rVB	124447	126110	21.99%	2.696%
2	1.571	157	165	178	rBV	107317	122279	21.32%	2.614%
3	2.111	323	333	351	rVB	221972	322047	56.15%	6.885%
4	2.513	450	458	470	rVB3	4183	6308	1.10%	0.135%
5	3.908	880	892	924	rBV2	34277	131486	22.92%	2.811%
6	4.352	1014	1030	1060	rBV2	99793	252703	44.06%	5.403%
7	5.050	1231	1247	1278	rBV2	231688	573562	100.00%	12.262%
8	5.619	1408	1424	1449	rBV	183256	373983	65.20%	7.995%
9	5.915	1507	1516	1532	rVB7	4822	10793	1.88%	0.231%
10	6.069	1550	1564	1588	rBV	127455	265251	46.25%	5.671%
11	6.989	1839	1850	1876	rBV	54006	103890	18.11%	2.221%
12	7.317	1940	1952	1970	rBV	283959	492800	85.92%	10.536%
13	7.625	2039	2048	2069	rBV2	28015	54587	9.52%	1.167%
14	8.091	2183	2193	2232	rBV	172271	364146	63.49%	7.785%
15	8.850	2418	2429	2450	rBV	289614	482636	84.15%	10.318%
16	10.217	2842	2854	2869	rBV	75128	119203	20.78%	2.548%
17	11.246	3164	3174	3195	rBV	304541	473595	82.57%	10.125%
18	11.622	3280	3291	3305	rBV	247257	384179	66.98%	8.213%
19	12.252	3478	3487	3496	rVB	5395	8293	1.45%	0.177%
20	14.037	4032	4042	4054	rBV	5759	9635	1.68%	0.206%




Sum of corrected areas: 4677486

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025491.D
Acq On : 13 Apr 2022 13:39
Operator : SY/MD
Sample : N2319-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

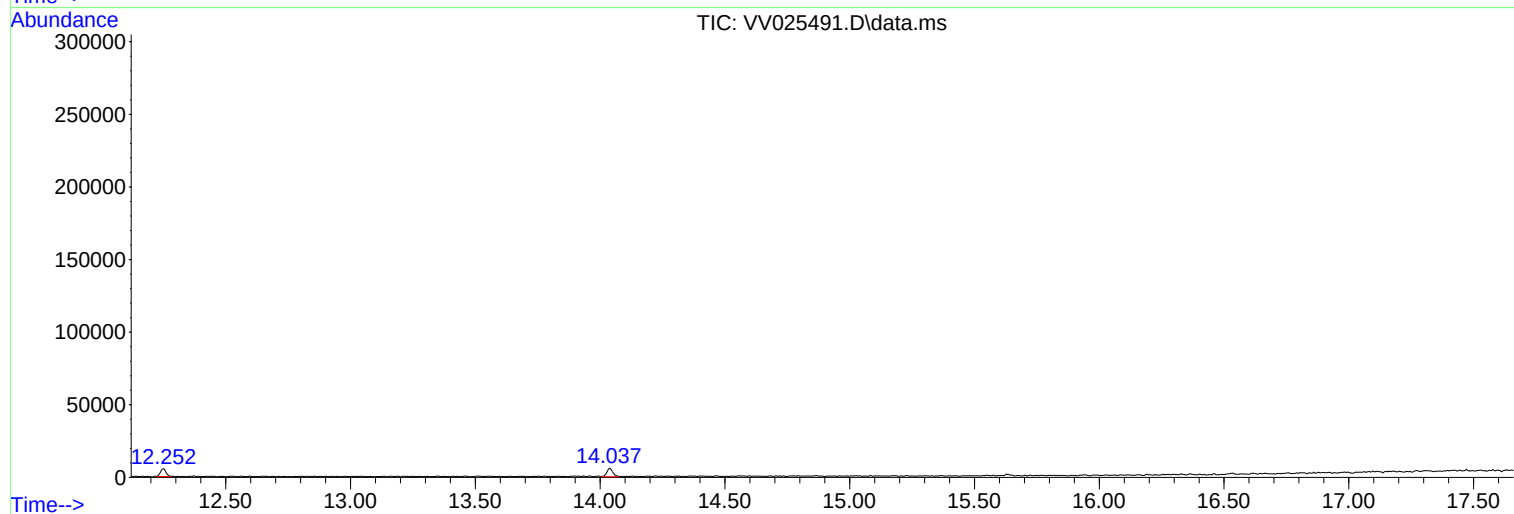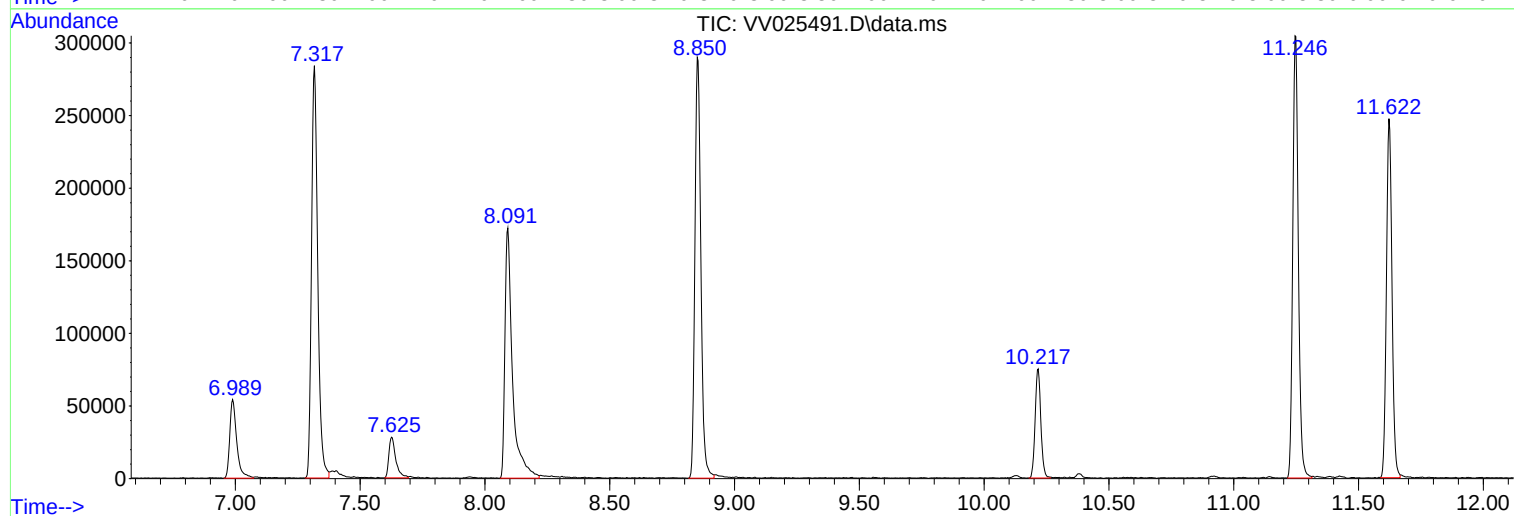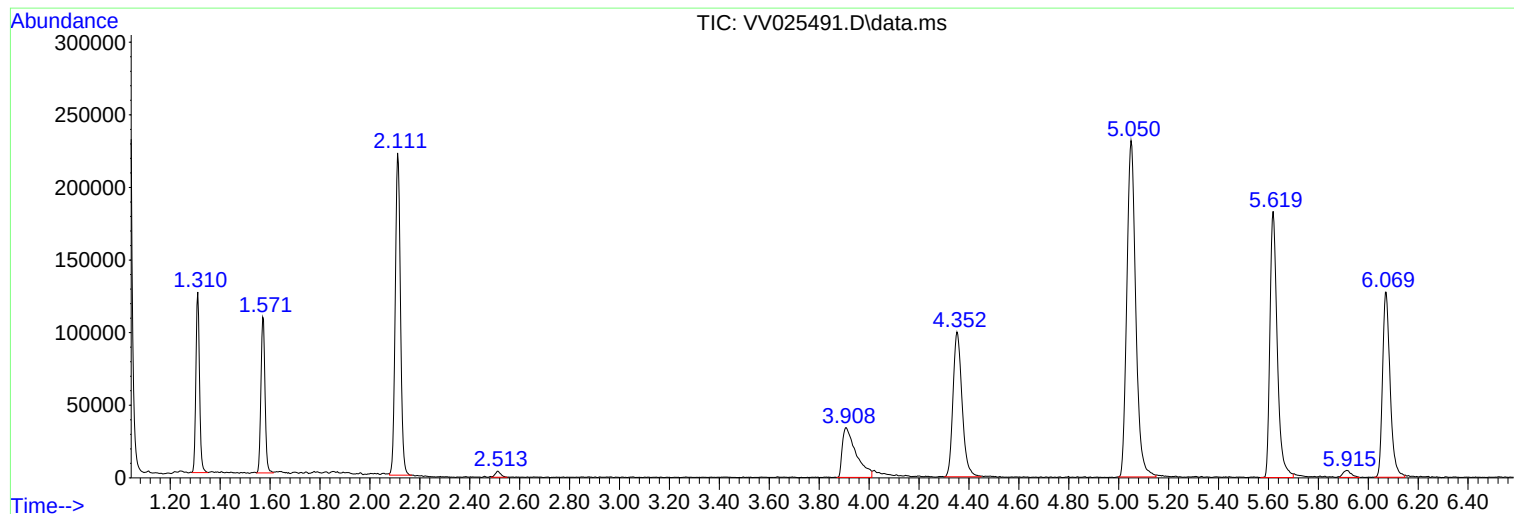

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025491.D
Acq On : 13 Apr 2022 13:39
Operator : SY/MD
Sample : N2319-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025491.D
Acq On : 13 Apr 2022 13:39
Operator : SY/MD
Sample : N2319-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc