

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
 Data File : VV025508.D
 Acq On : 13 Apr 2022 22:14
 Operator : SY/MD
 Sample : N2357-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAZ14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	93	rVB	82004	84384	18.90%	2.343%
2	1.571	158	165	177	rBV	80661	89358	20.01%	2.481%
3	2.111	322	333	351	rVB	148983	218315	48.89%	6.062%
4	3.902	880	890	923	rBV	36922	131921	29.54%	3.663%
5	4.352	1015	1030	1063	rBV	79699	204186	45.73%	5.669%
6	5.050	1231	1247	1274	rBV4	176777	446519	100.00%	12.398%
7	5.619	1413	1424	1447	rBV	132999	276624	61.95%	7.681%
8	5.921	1506	1518	1534	rVB8	7952	18332	4.11%	0.509%
9	6.072	1552	1565	1590	rBV2	102070	216814	48.56%	6.020%
10	6.989	1841	1850	1873	rBV	33184	65356	14.64%	1.815%
11	7.317	1941	1952	1971	rBV	197578	351578	78.74%	9.762%
12	7.625	2038	2048	2070	rBV2	18775	35658	7.99%	0.990%
13	7.937	2135	2145	2157	rBV3	7137	13005	2.91%	0.361%
14	8.091	2183	2193	2226	rBV	156151	329334	73.76%	9.144%
15	8.854	2417	2430	2454	rBV	215869	359075	80.42%	9.970%
16	10.217	2843	2854	2867	rBV	67304	107698	24.12%	2.990%
17	10.381	2894	2905	2916	rBV4	13585	21738	4.87%	0.604%
18	11.246	3164	3174	3198	rBV	212610	331618	74.27%	9.208%
19	11.622	3280	3291	3309	rBV	184202	290902	65.15%	8.077%
20	12.246	3474	3485	3496	rVB3	5756	9115	2.04%	0.253%




Sum of corrected areas: 3601530

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025508.D
Acq On : 13 Apr 2022 22:14
Operator : SY/MD
Sample : N2357-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

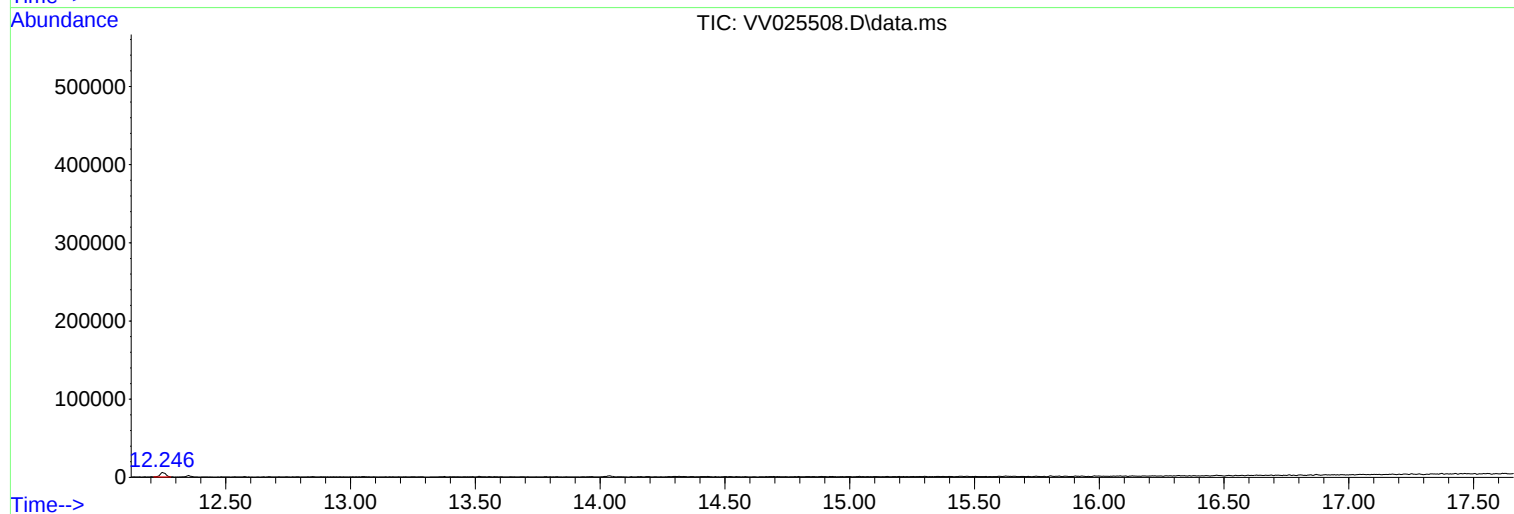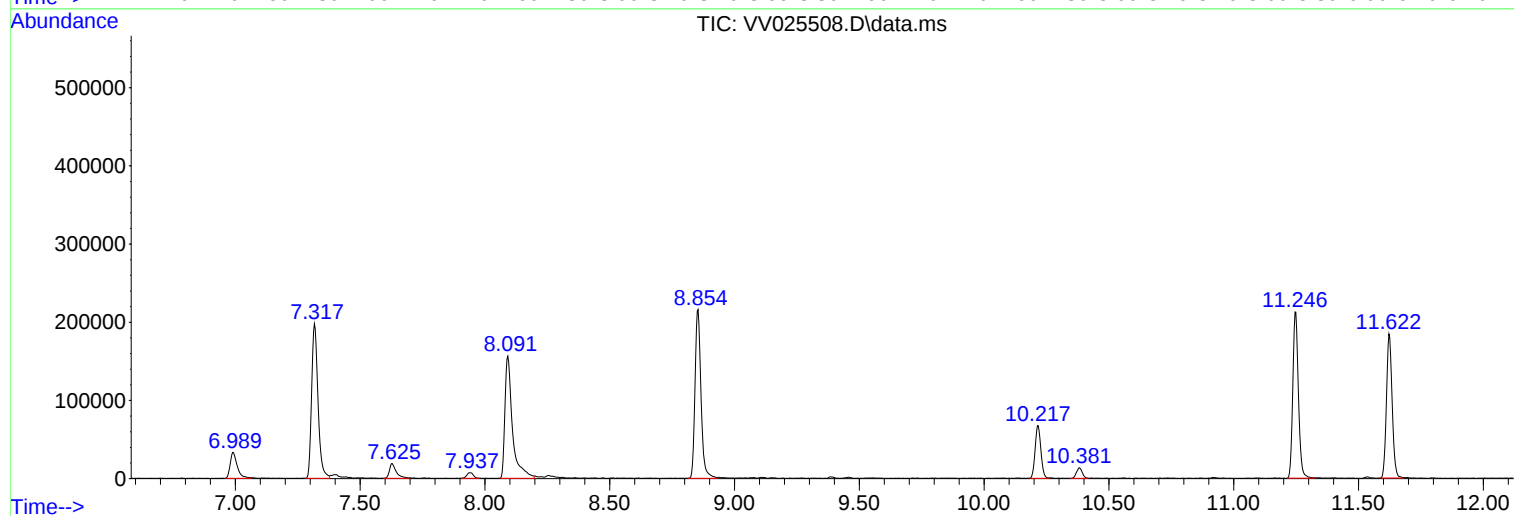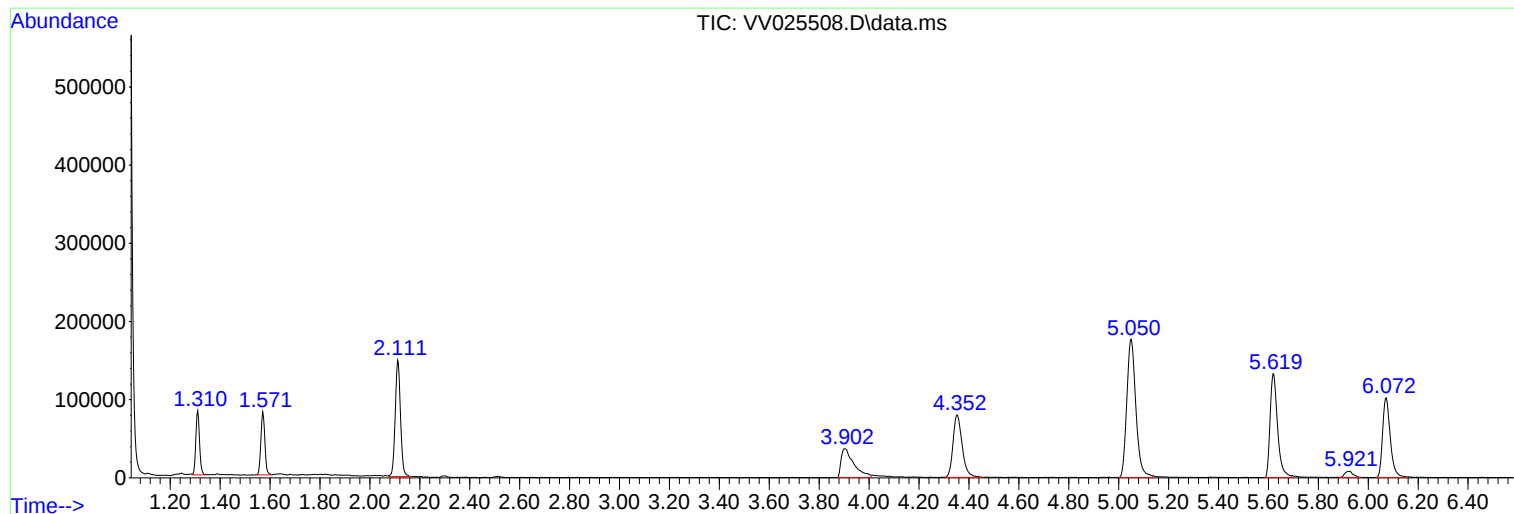

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025508.D
Acq On : 13 Apr 2022 22:14
Operator : SY/MD
Sample : N2357-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
Data File : VV025508.D
Acq On : 13 Apr 2022 22:14
Operator : SY/MD
Sample : N2357-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAZ14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
