
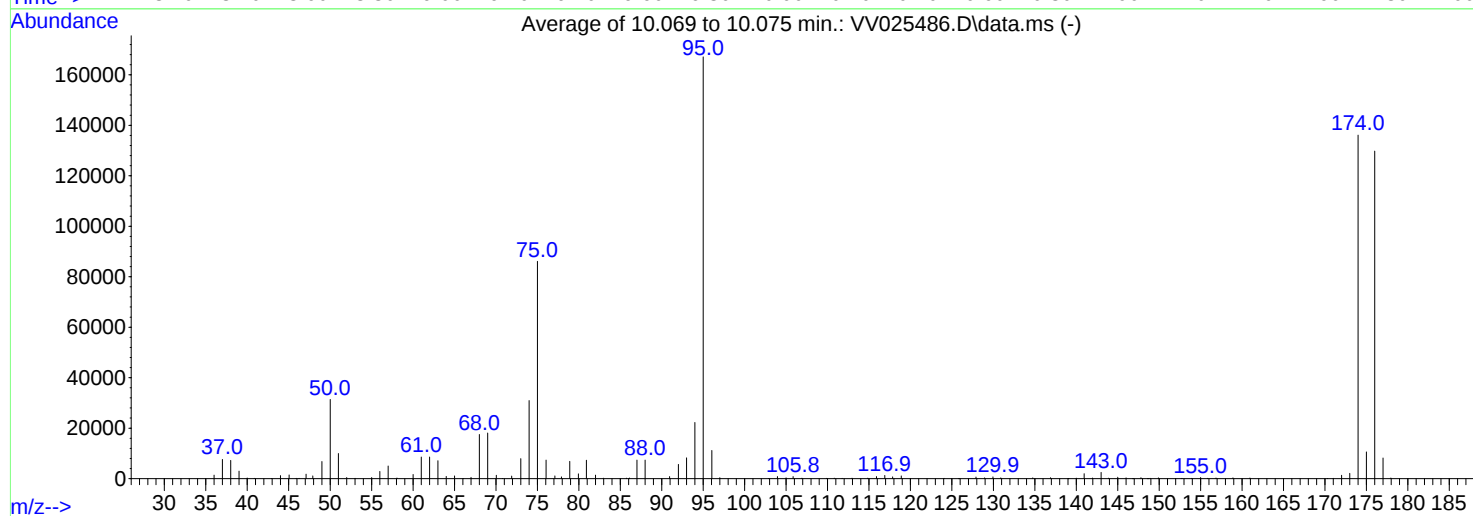


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041322\
 Data File : VV025486.D
 Acq On : 13 Apr 2022 10:37
 Operator : SY/MD
 Sample : BFB301
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB301

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Apr 19 05:06:28 2022

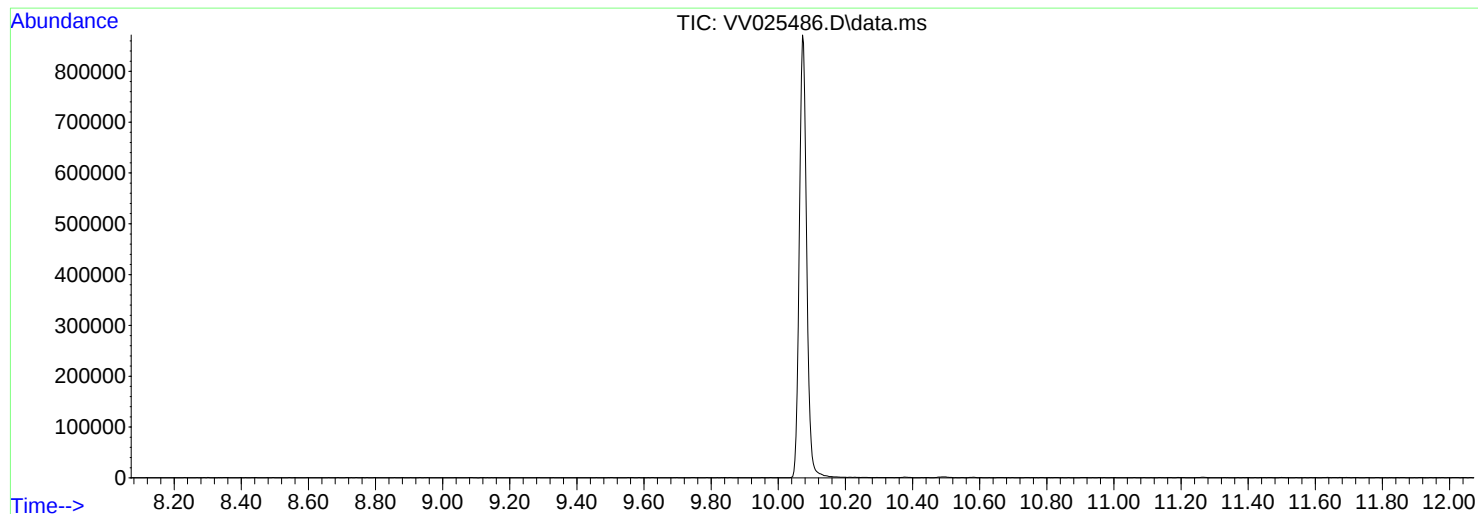

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	31355	PASS
75	95	30	80	51.5	86091	PASS
95	95	100	100	100.0	167125	PASS
96	95	5	9	6.7	11176	PASS
173	174	0.00	2	1.5	2079	PASS
174	95	50	120	81.4	136099	PASS
175	174	5	9	7.8	10587	PASS
176	174	95	105	95.4	129773	PASS
177	176	5	10	6.3	8212	PASS

m/z	Abundance
44.00	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
36.00	1329.0
37.00	7489.0
38.00	7082.0
39.00	2877.0
40.00	225.0
40.90	100.0
44.00	1508.0
45.00	1361.0
46.30	280.0
47.10	2005.0
47.90	953.0
49.00	6757.0
50.00	30176.0
51.00	9472.0
52.00	477.0
53.00	134.0
55.00	455.0
56.00	2589.0
57.00	4922.0
58.00	251.0
60.00	1696.0
61.00	8272.0
62.00	8039.0
63.00	6951.0
64.00	916.0
65.00	1072.0
66.00	144.0
67.00	459.0
68.00	16824.0
69.00	17328.0
70.00	1334.0
70.80	138.0
71.90	972.0
73.00	7425.0
74.00	29056.0
75.00	81832.0
76.00	7381.0
77.10	966.0
78.00	616.0
78.90	6624.0
79.90	1863.0
80.90	6935.0
82.00	1405.0
82.90	139.0
85.70	184.0
86.10	238.0
87.00	6909.0
88.00	6978.0
91.00	784.0
92.00	5321.0
93.00	7676.0
94.00	21280.0
95.00	157824.0
96.10	10327.0
97.00	367.0
102.90	125.0
104.00	765.0
105.00	313.0
105.90	823.0
106.90	237.0
109.90	138.0
110.80	185.0
111.80	131.0
113.00	183.0
114.80	213.0
115.90	769.0
116.90	1146.0
117.80	587.0
118.90	1032.0
124.00	101.0
125.80	104.0
127.90	605.0
129.00	330.0
130.00	573.0
130.90	324.0
134.70	278.0
136.90	368.0
140.00	156.0
141.00	1946.0
141.90	274.0
143.00	2299.0
143.90	221.0
145.00	537.0
146.00	324.0
147.80	360.0
148.60	112.0
149.00	114.0
149.90	266.0
152.00	124.0
152.70	125.0
153.90	140.0
155.00	373.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

155.80	112.0
156.80	238.0
158.90	289.0
161.00	228.0
172.00	1247.0
173.00	1952.0
174.00	126056.0
175.00	9953.0
176.00	119752.0
177.00	7811.0
178.00	286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
36.00	1459.0
37.00	7909.0
38.00	7568.0
39.00	3078.0
40.00	293.0
40.80	126.0
43.00	102.0
44.00	1500.0
45.10	1549.0
45.90	227.0
47.10	1816.0
47.90	1102.0
49.00	7046.0
50.00	32560.0
51.00	10296.0
52.00	468.0
53.00	124.0
55.00	482.0
56.00	2962.0
57.00	5214.0
58.10	264.0
60.00	1732.0
61.00	8931.0
62.00	8826.0
63.00	7307.0
64.00	956.0
65.00	1109.0
66.10	113.0
67.00	522.0
68.00	18168.0
69.00	18880.0
70.00	1397.0
71.90	1040.0
73.00	8249.0
74.00	32144.0
75.00	89448.0
76.00	7614.0
77.10	1185.0
77.90	709.0
78.90	7168.0
80.00	2012.0
80.90	7574.0
82.00	1430.0
82.90	196.0
85.80	221.0
86.10	279.0
87.00	7646.0
88.00	7562.0
91.00	844.0
92.00	5976.0
93.00	8546.0
94.00	23120.0
95.00	173632.0
96.00	11636.0
97.00	416.0
102.90	102.0
103.90	850.0
105.00	320.0
105.90	905.0
106.90	220.0
109.90	164.0
110.80	222.0
111.80	142.0
112.90	199.0
114.80	207.0
115.90	840.0
116.90	1313.0
117.90	726.0
118.90	1069.0
124.00	139.0
127.90	673.0
128.90	313.0
129.90	706.0
130.90	349.0
134.80	359.0
136.90	433.0
139.00	107.0
140.00	181.0
141.00	2067.0
142.00	305.0
143.00	2552.0
143.90	224.0
145.00	629.0
146.00	371.0
147.80	391.0
148.90	118.0
149.90	319.0
152.00	125.0
152.70	137.0
154.00	162.0
155.00	458.0
155.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

156.80	234.0
158.90	357.0
161.00	240.0
170.30	143.0
171.00	234.0
172.00	1351.0
173.00	2176.0
174.00	141312.0
175.00	11019.0
176.00	134272.0
177.00	8550.0
178.00	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
36.00	1463.0
37.00	7522.0
38.00	7029.0
39.00	3064.0
40.00	327.0
40.80	124.0
42.90	119.0
44.00	1390.0
45.10	1557.0
45.90	196.0
46.20	173.0
47.10	1456.0
47.90	1116.0
49.00	6527.0
50.00	31328.0
51.00	10100.0
52.00	441.0
53.00	100.0
55.00	466.0
56.00	2979.0
57.00	4977.0
58.10	241.0
60.00	1557.0
61.00	8517.0
62.00	8864.0
63.00	7049.0
64.00	879.0
65.00	1098.0
67.00	499.0
68.00	17568.0
69.00	18080.0
70.10	1370.0
71.90	979.0
73.00	8096.0
74.00	31648.0
75.00	86992.0
76.10	7106.0
77.10	1173.0
77.80	711.0
78.90	6855.0
80.00	1927.0
80.90	7286.0
82.00	1334.0
83.00	217.0
85.80	252.0
86.10	283.0
87.00	7430.0
88.00	7496.0
90.90	779.0
92.00	5740.0
93.00	8578.0
94.00	22424.0
95.00	169920.0
96.00	11565.0
97.00	412.0
103.90	799.0
105.00	265.0
105.80	855.0
106.90	189.0
109.90	147.0
110.80	236.0
111.70	146.0
112.90	195.0
114.90	208.0
115.90	842.0
116.90	1303.0
117.90	766.0
118.90	1073.0
124.10	161.0
127.90	648.0
129.00	277.0
129.90	747.0
130.90	321.0
134.80	386.0
136.90	444.0
140.00	183.0
140.90	1978.0
142.00	272.0
143.00	2538.0
143.90	181.0
145.00	553.0
146.00	327.0
146.80	102.0
147.80	406.0
148.80	124.0
149.90	297.0
152.80	133.0
154.00	164.0
155.00	486.0
155.90	117.0
156.90	267.0
158.90	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

160.90	216.0
170.30	145.0
171.00	217.0
172.00	1369.0
173.00	2109.0
174.00	140928.0
175.00	10790.0
176.00	135296.0
177.00	8274.0
177.90	275.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301