




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
 Data File : VV025554.D
 Acq On : 14 Apr 2022 18:25
 Operator : SY/MD
 Sample : N2384-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R3

Manual IntegrationsAPPROVED

Quant Time: Apr 15 07:25:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 15 07:05:00 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/15/2022
 Supervised By :Mahesh Dadoda 04/19/2022

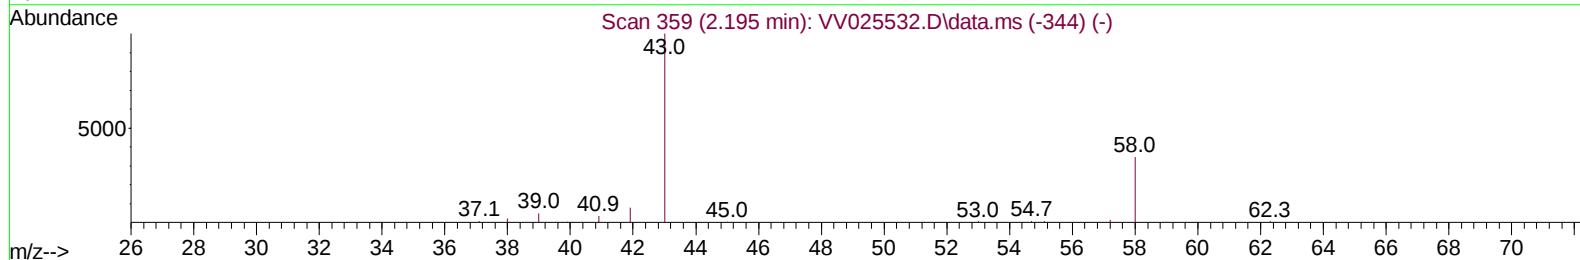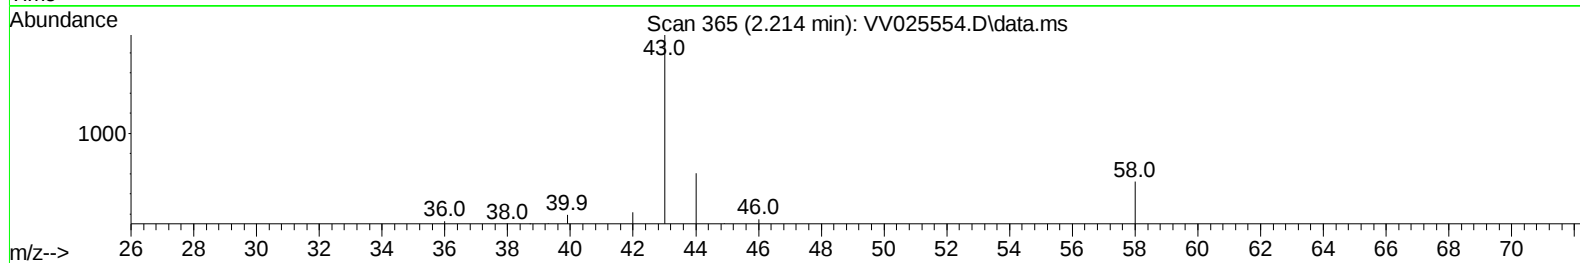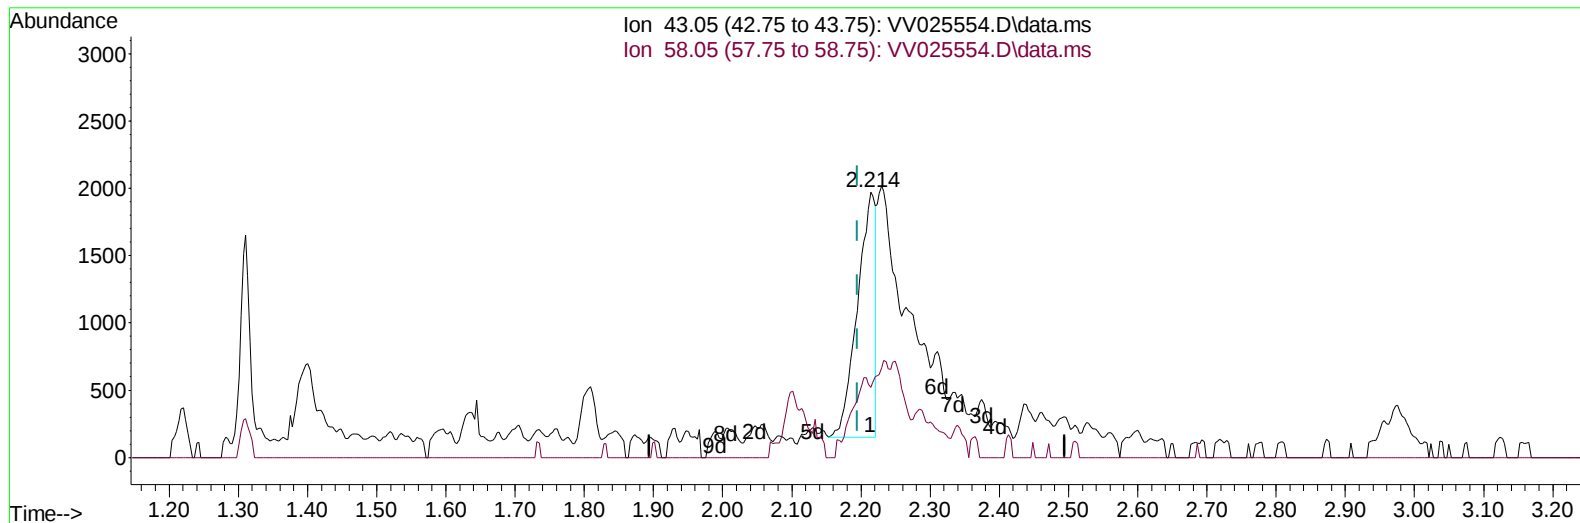

TIC: VV025554.D\data.ms

(13) Acetone (T)

2.214min (+ 0.019) 3.50 ug/L

response 3235

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	34.59
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
 Data File : VV025554.D
 Acq On : 14 Apr 2022 18:25
 Operator : SY/MD
 Sample : N2384-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R3

Manual IntegrationsAPPROVED

Quant Time: Apr 15 07:25:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 15 07:05:00 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/15/2022
 Supervised By :Mahesh Dadoda 04/19/2022

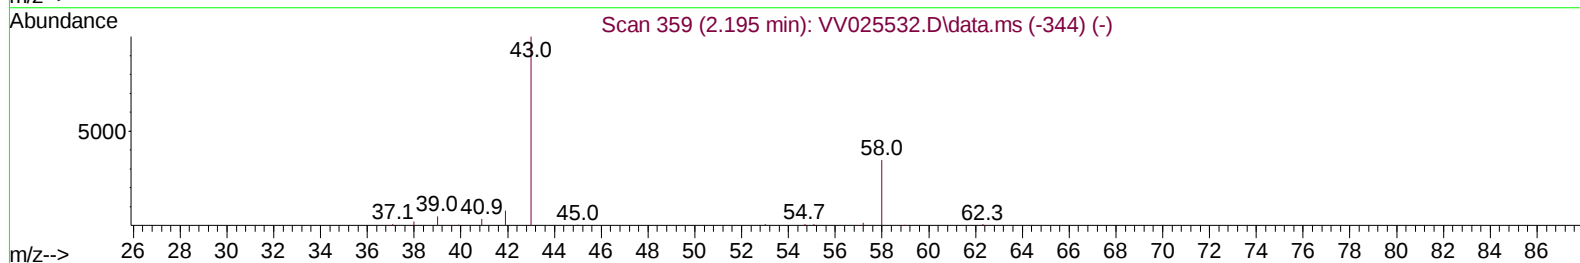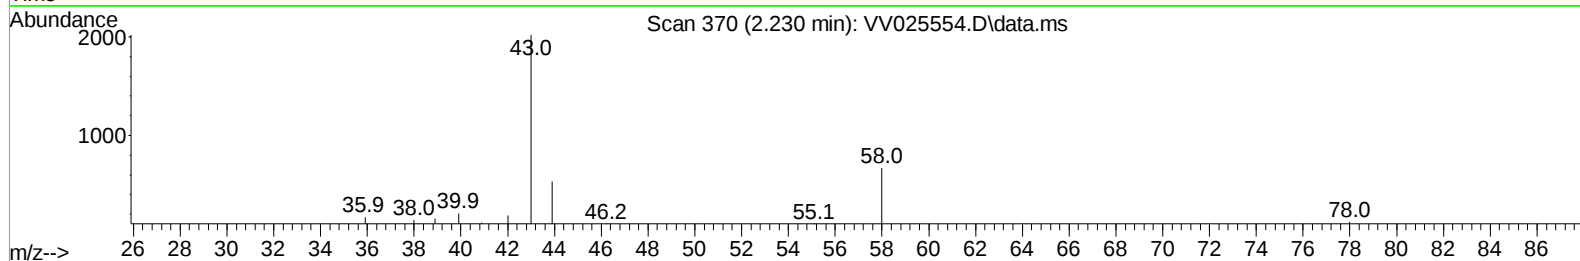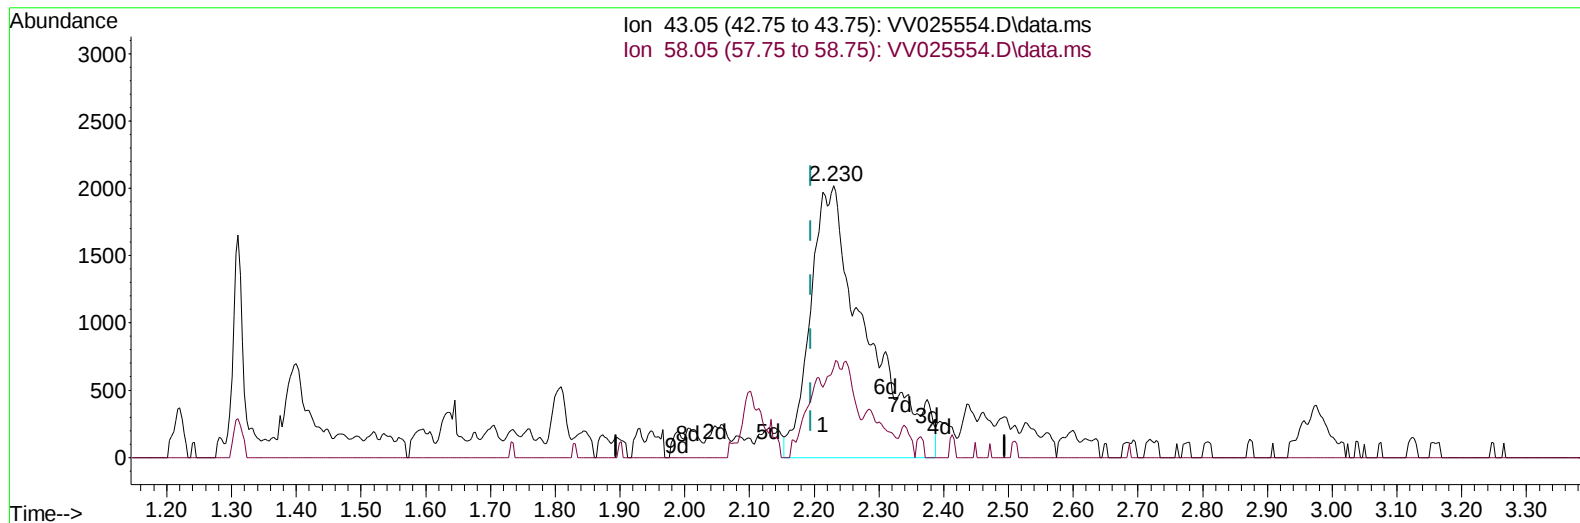

TIC: VV025554.D\data.ms

(13) Acetone (T)

2.230min (+ 0.035) 13.17 ug/L m

response 12182

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	9.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
 Data File : VV025554.D
 Acq On : 14 Apr 2022 18:25
 Operator : SY/MD
 Sample : N2384-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6R3

Manual IntegrationsAPPROVED

Quant Time: Apr 15 07:25:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 15 07:05:00 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/15/2022
 Supervised By :Mahesh Dadoda 04/19/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	120498	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125924	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63439	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60836	5.430	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	108.600%	
7) Chloroethane-d5	1.571	69	54604	4.582	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.600%	
11) 1,1-Dichloroethene-d2	2.111	63	92096	4.104	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	82.000%	
20) 2-Butanone-d5	3.924	46	57297	42.046	ug/L	0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	84.100%	
24) Chloroform-d	4.355	84	85740	5.065	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	5.040	65	39496	5.415	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.200%	
32) Benzene-d6	5.053	84	163003	4.474	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.400%	
36) 1,2-Dichloropropane-d6	6.072	67	49503	4.872	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.400%	
41) Toluene-d8	7.316	98	139236	4.118	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	7.628	79	15210	4.453	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.091	63	52929	44.157	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.320%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	31169	4.855	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	52632	4.948	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.000%	
Target Compounds						
					Qvalue	
13) Acetone	2.230	43	12182m	13.171	ug/L	
16) Methylene chloride	2.513	84	4372	0.431	ug/L	92
25) Chloroform	4.381	83	27779	1.774	ug/L	98
38) Bromodichloromethane	6.516	83	3975	0.372	ug/L #	93
40) 4-Methyl-2-pentanone	7.239	43	9220	2.676	ug/L #	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025554.D
Acq On : 14 Apr 2022 18:25
Operator : SY/MD
Sample : N2384-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6R3

Manual IntegrationsAPPROVED

Quant Time: Apr 15 07:25:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 15 07:05:00 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/15/2022
Supervised By :Mahesh Dadoda 04/19/2022

