

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041422\
 Data File : VW025540.D
 Acq On : 14 Apr 2022 12:56
 Operator : SY/MD
 Sample : N2356-08DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDS6DL

Quant Time: Apr 15 07:22:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 15 07:05:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	140460	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	137090	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61778	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	64760	4.959	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	99.200%	
7) Chloroethane-d5	1.571	69	61531	4.429	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.600%	
11) 1,1-Dichloroethene-d2	2.114	63	95184	3.639	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.800%	
20) 2-Butanone-d5	3.899	46	86385	54.383	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	108.760%	
24) Chloroform-d	4.352	84	99556	5.045	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.037	65	45938	5.403	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.000%	
32) Benzene-d6	5.053	84	197422	4.977	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.600%	
36) 1,2-Dichloropropane-d6	6.072	67	59378	5.368	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.400%	
41) Toluene-d8	7.317	98	162439	4.413	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.200%	
43) trans-1,3-Dichloroprop...	7.629	79	16883	4.541	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.800%	
46) 2-Hexanone-d5	8.088	63	61349	47.012	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.020%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35360	5.060	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	53503	5.166	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	103.400%	
Target Compounds					Qvalue	
30) Cyclohexane	4.683	56	1691	0.115	ug/L	# 62
33) Benzene	5.101	78	115907	2.862	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025540.D
Acq On : 14 Apr 2022 12:56
Operator : SY/MD
Sample : N2356-08DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDS6DL

Quant Time: Apr 15 07:22:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 15 07:05:00 2022
Response via : Initial Calibration




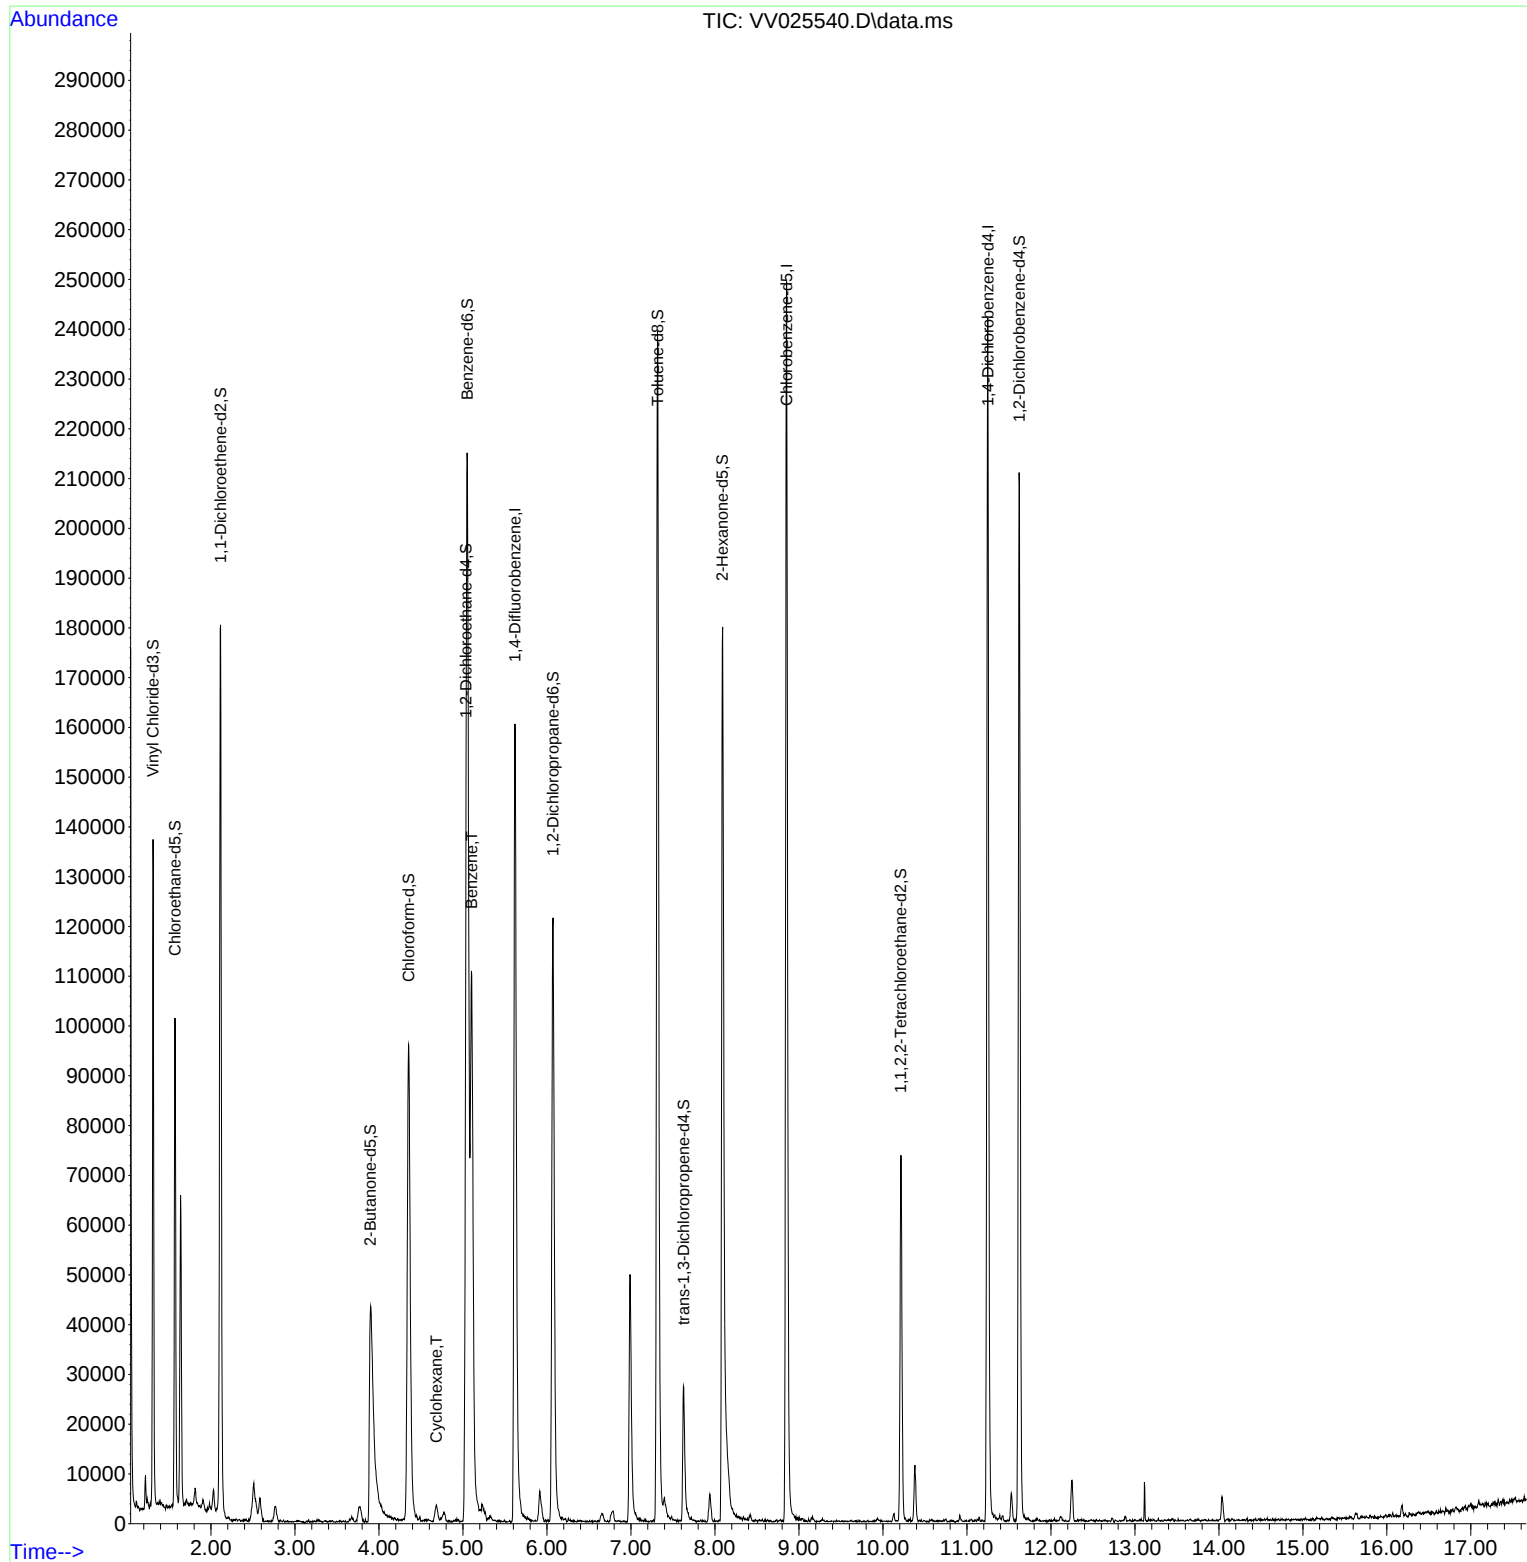


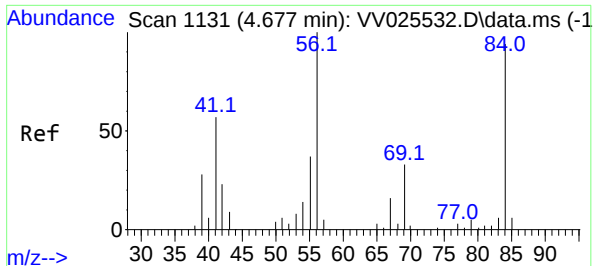

#30
Cyclohexane
Concen: 0.115 ug/L
RT: 4.683 min Scan# 1131
Delta R.T. 0.006 min
Lab File: VV025540.D
Acq: 14 Apr 2022 12:56

Instrument :
MSVOA_V
ClientSampleId :
GBDS6DL

Tgt Ion: 56 Resp: 1691
Ion Ratio Lower Upper
56 100
69 33.7 26.1 39.1
84 49.4 78.6 118.0#

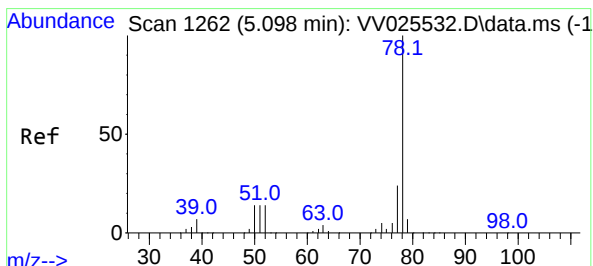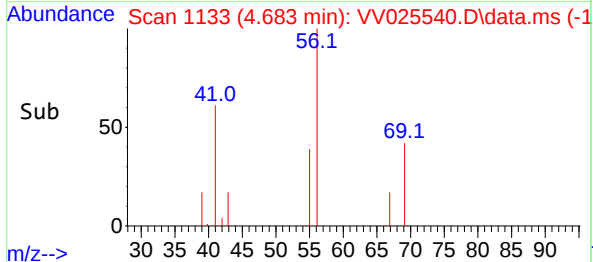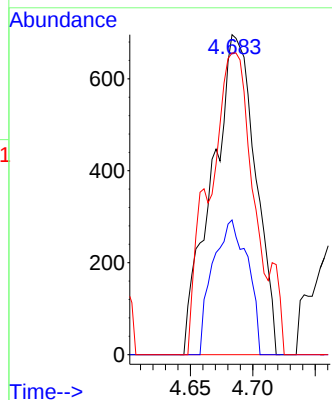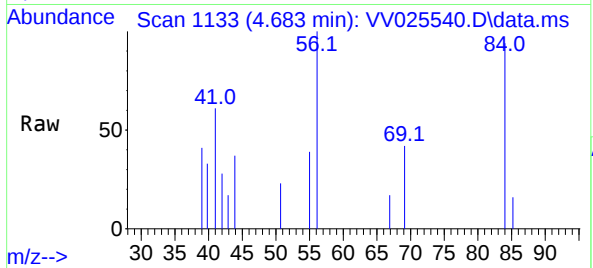

#33
Benzene
Concen: 2.862 ug/L
RT: 5.101 min Scan# 1263
Delta R.T. 0.003 min
Lab File: VV025540.D
Acq: 14 Apr 2022 12:56

Tgt Ion: 78 Resp: 115907

