

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041422\
 Data File : VW025547.D
 Acq On : 14 Apr 2022 15:40
 Operator : SY/MD
 Sample : N2356-19DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDT7DL

Quant Time: Apr 15 07:23:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 15 07:05:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	130805	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	131789	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57604	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	55524	4.566	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.400%	
7) Chloroethane-d5	1.571	69	54334	4.200	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	84.000%	
11) 1,1-Dichloroethene-d2	2.111	63	84959	3.487	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.800%	
20) 2-Butanone-d5	3.899	46	72806	49.217	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.440%	
24) Chloroform-d	4.352	84	86639	4.715	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.037	65	40286	5.088	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.800%	
32) Benzene-d6	5.056	84	168958	4.431	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.600%	
36) 1,2-Dichloropropane-d6	6.072	67	50711	4.769	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.400%	
41) Toluene-d8	7.317	98	139825	3.951	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.000%	
43) trans-1,3-Dichloroprop...	7.625	79	14133	3.954	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.000%	
46) 2-Hexanone-d5	8.091	63	53870	42.942	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.880%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30645	4.561	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	44840	4.643	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.800%	
Target Compounds						
					Qvalue	
22) cis-1,2-Dichloroethene	3.918	96	15524	1.551	ug/L	96
34) Trichloroethene	5.915	95	80361	7.774	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025547.D
Acq On : 14 Apr 2022 15:40
Operator : SY/MD
Sample : N2356-19DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDT7DL

Quant Time: Apr 15 07:23:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 15 07:05:00 2022
Response via : Initial Calibration




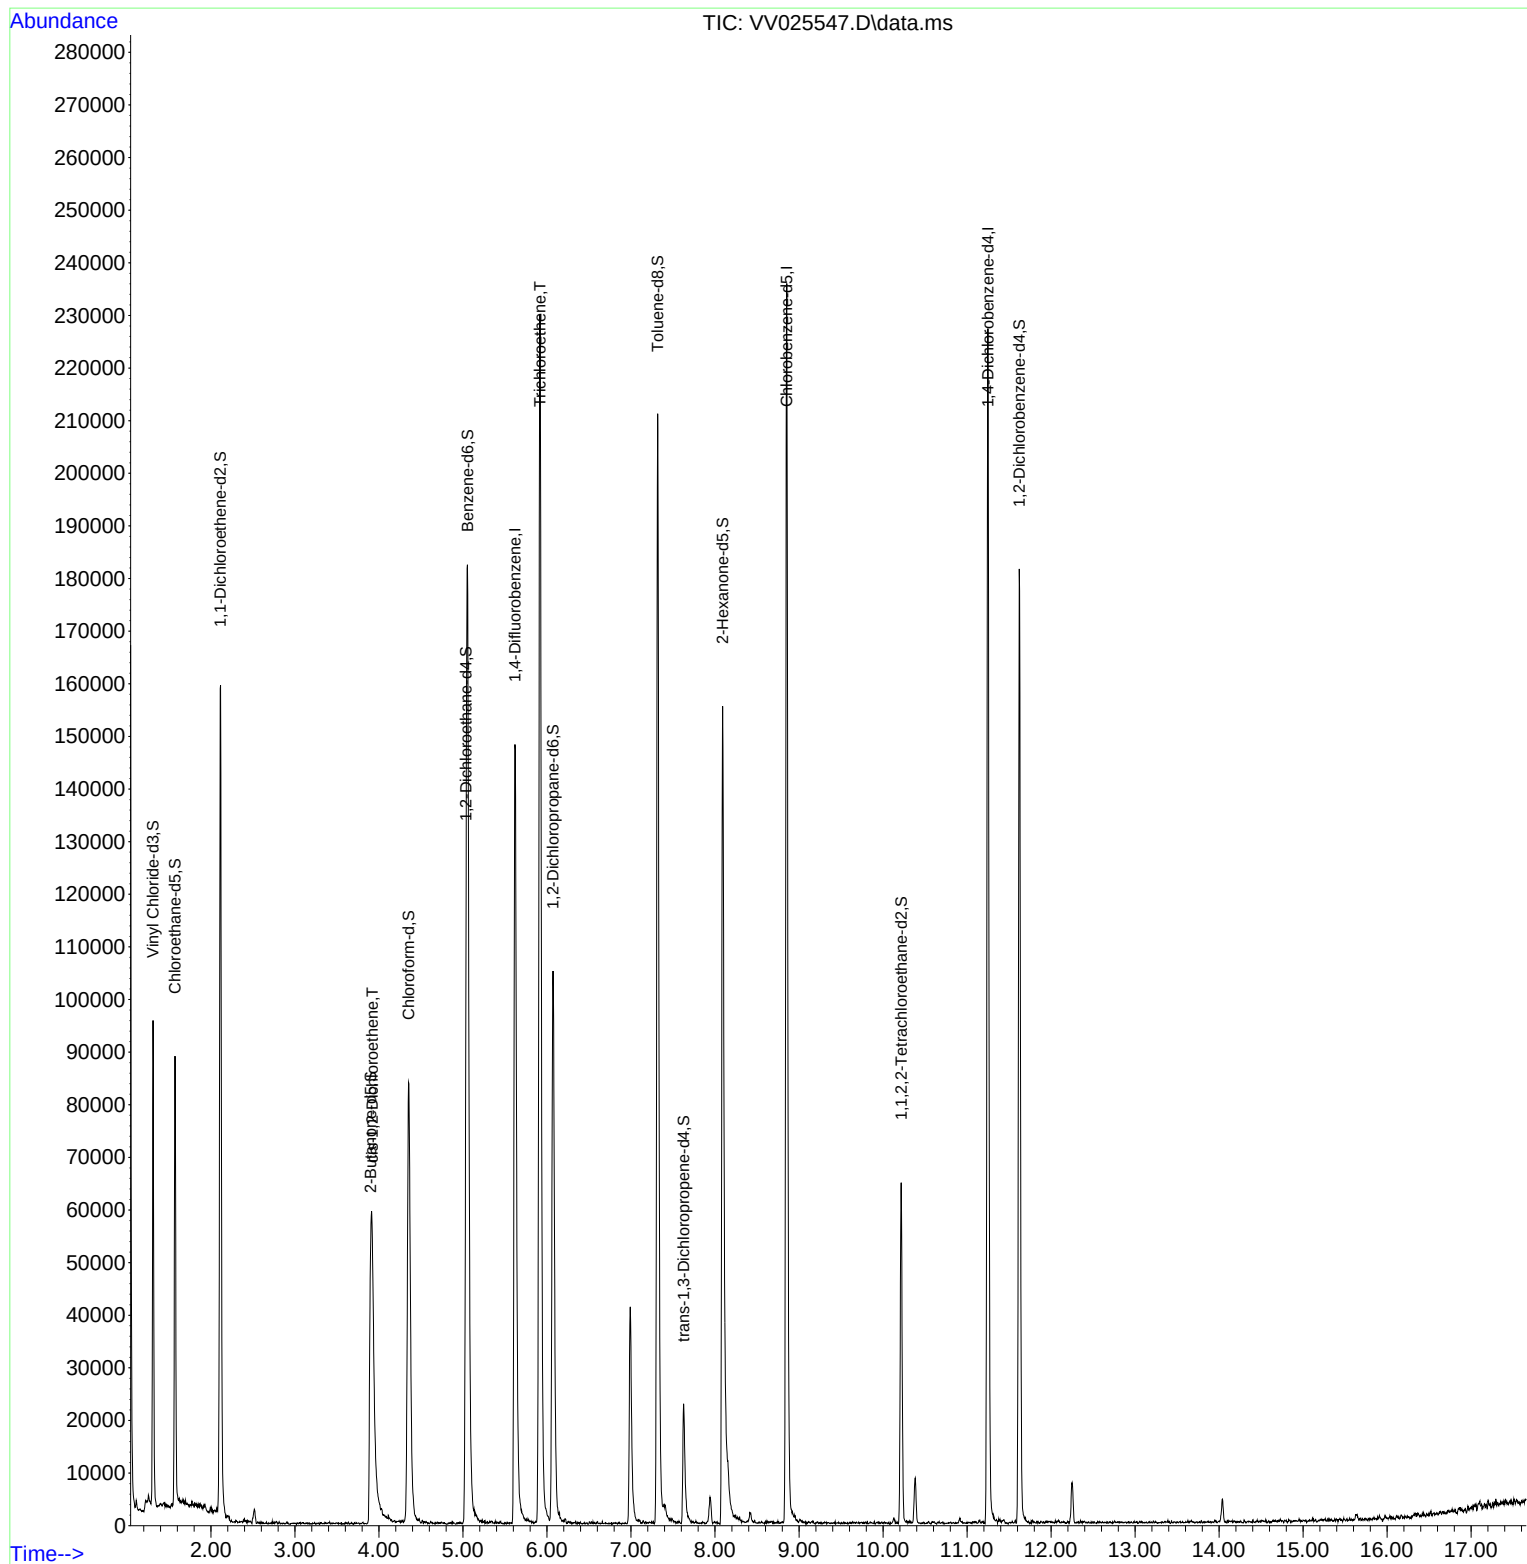


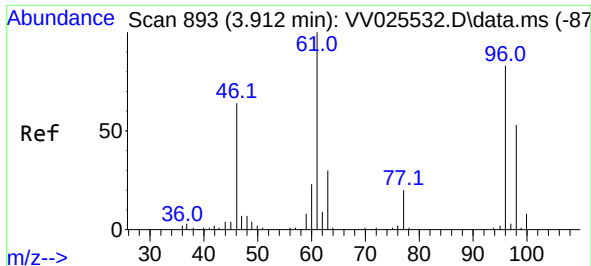

#22
 cis-1,2-Dichloroethene
 Concen: 1.551 ug/L
 RT: 3.918 min Scan# 894
 Delta R.T. 0.006 min
 Lab File: VV025547.D
 Acq: 14 Apr 2022 15:40

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDT7DL

Tgt Ion: 96 Resp: 15524
 Ion Ratio Lower Upper
 96 100
 61 110.4 80.0 148.6
 68 0.0 0.0 0.0

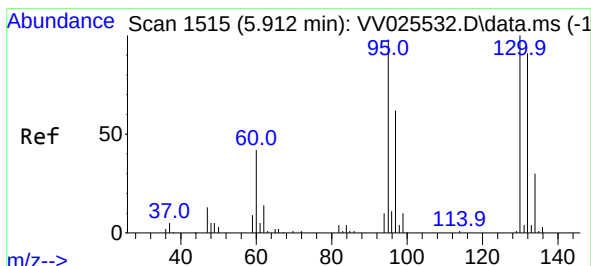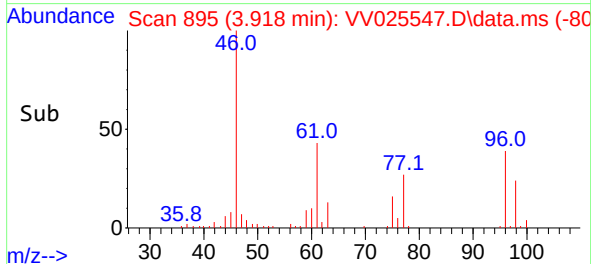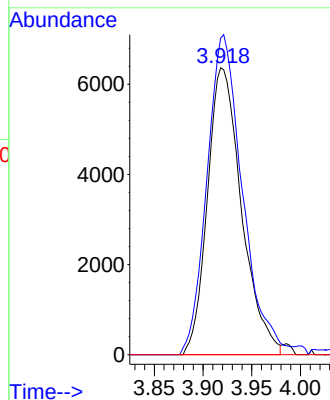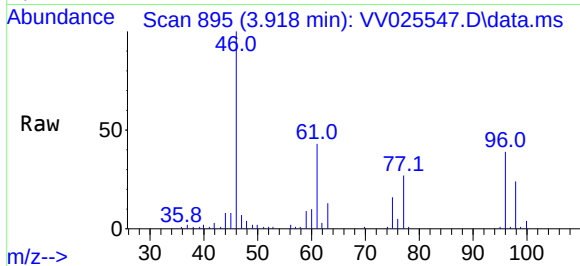

#34
 Trichloroethene
 Concen: 7.774 ug/L
 RT: 5.915 min Scan# 1516
 Delta R.T. 0.003 min
 Lab File: VV025547.D
 Acq: 14 Apr 2022 15:40

Tgt Ion: 95 Resp: 80361
 Ion Ratio Lower Upper
 95 100
 97 63.6 45.8 85.2
 132 98.4 68.0 126.4
 130 101.3 71.9 133.5

