

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041422\
 Data File : VW025550.D
 Acq On : 14 Apr 2022 16:51
 Operator : SY/MD
 Sample : N2388-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE5

Quant Time: Apr 15 07:24:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 15 07:05:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	124887	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	130023	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56932	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	55772	4.803	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.000%
7) Chloroethane-d5	1.571	69	52485	4.249	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.000%
11) 1,1-Dichloroethene-d2	2.111	63	85243	3.665	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	3.902	46	80642	57.098	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.200%
24) Chloroform-d	4.355	84	85362	4.865	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
26) 1,2-Dichloroethane-d4	5.037	65	41851	5.536	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.800%
32) Benzene-d6	5.053	84	166223	4.418	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
36) 1,2-Dichloropropane-d6	6.072	67	50318	4.796	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.317	98	136905	3.921	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	7.625	79	14572	4.132	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.600%
46) 2-Hexanone-d5	8.091	63	55827	45.106	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.220%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29595	4.465	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	46026	4.822	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						
					Qvalue	
25) Chloroform	4.384	83	12635	0.779	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025550.D
Acq On : 14 Apr 2022 16:51
Operator : SY/MD
Sample : N2388-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFE5

Quant Time: Apr 15 07:24:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 15 07:05:00 2022
Response via : Initial Calibration

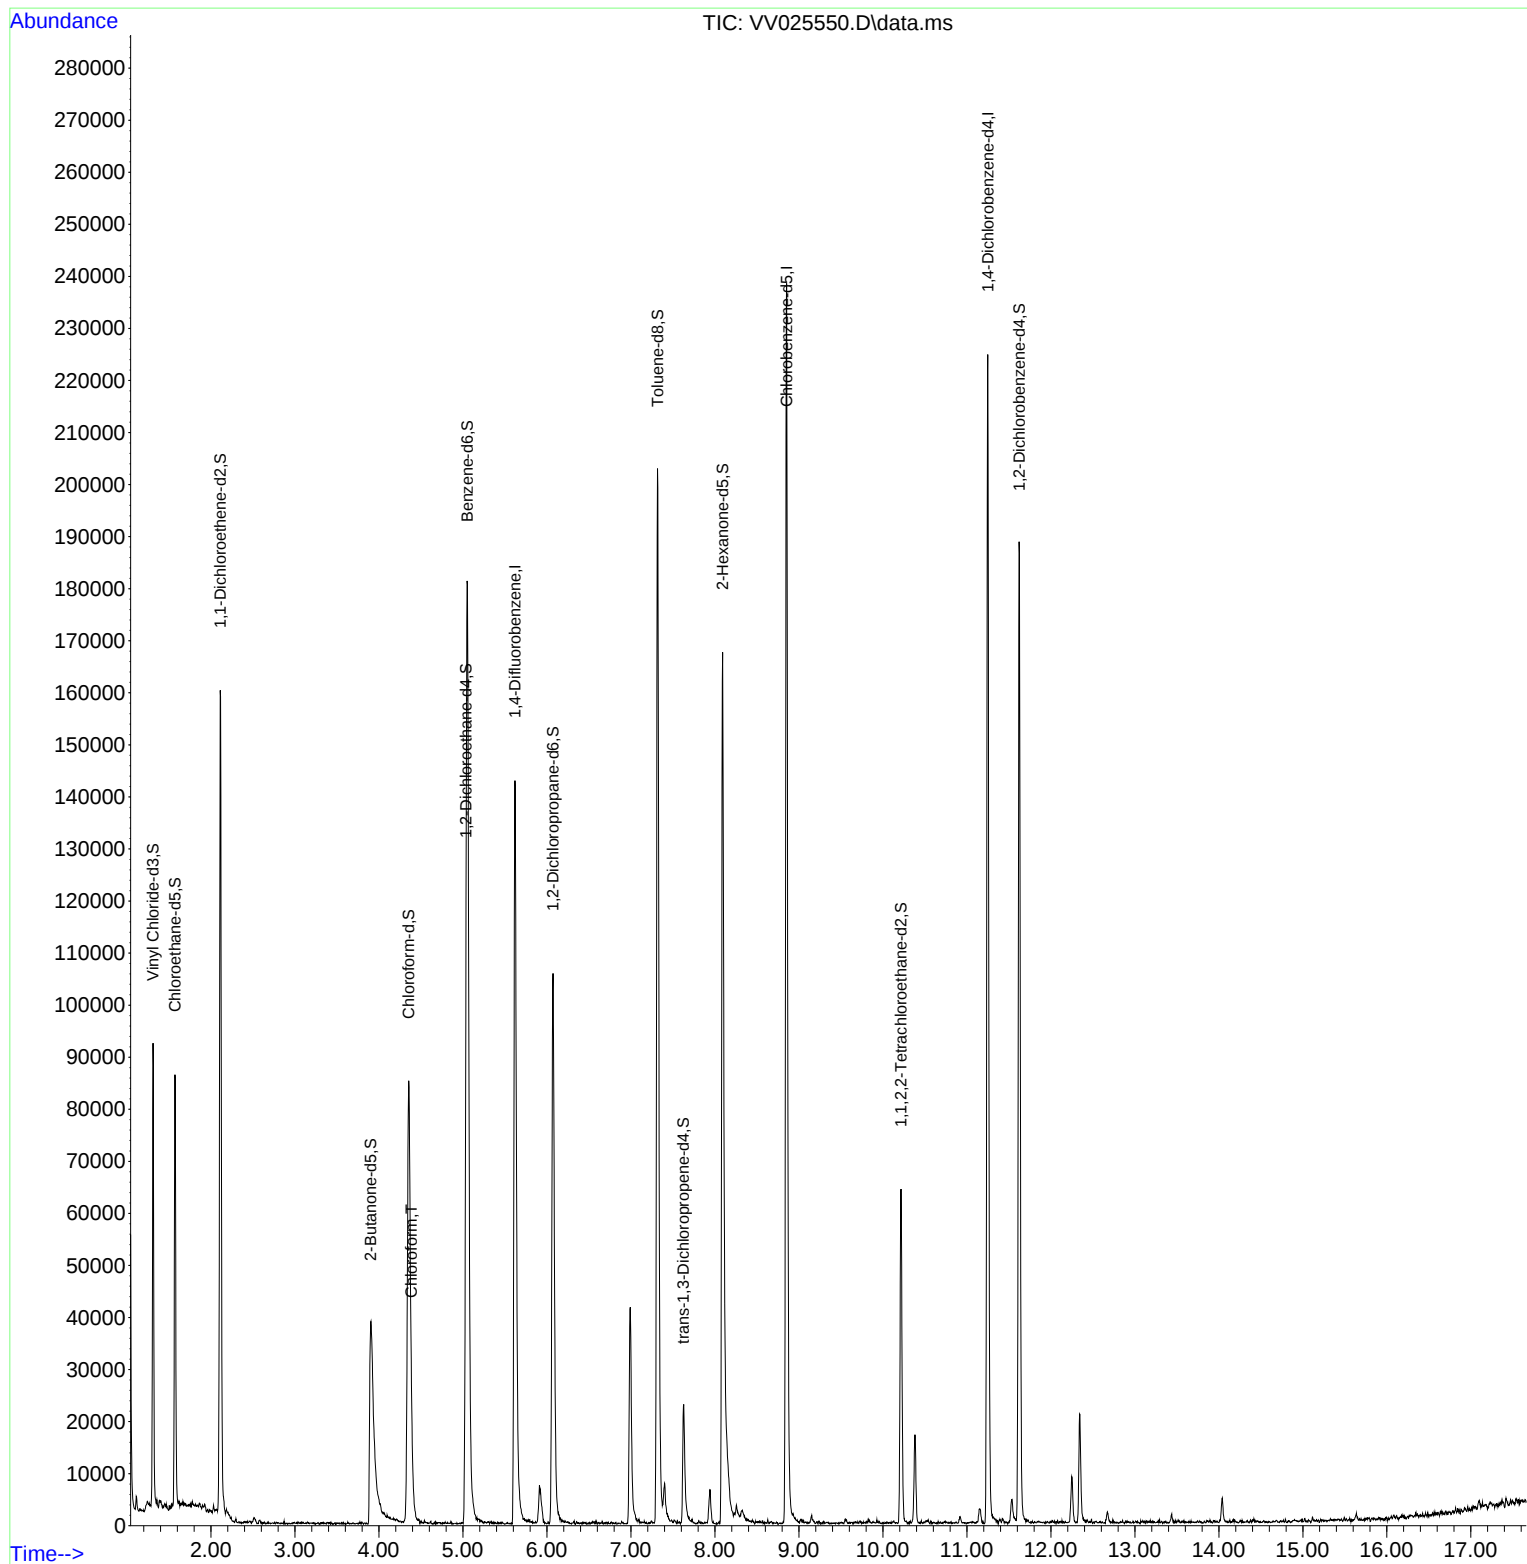

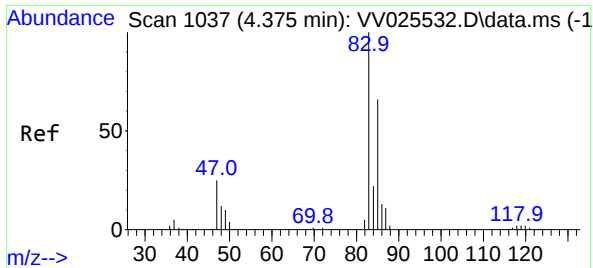

#25
Chloroform
Concen: 0.779 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.009 min
Lab File: VV025550.D
Acq: 14 Apr 2022 16:51

Instrument :
MSVOA_V
ClientSampleId :
BFFE5

Tgt Ion: 83 Resp: 12635
Ion Ratio Lower Upper
83 100
85 67.9 43.5 80.7

