

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041422\
 Data File : VW025551.D
 Acq On : 14 Apr 2022 17:14
 Operator : SY/MD
 Sample : N2388-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE6

Quant Time: Apr 15 07:24:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 15 07:05:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	141052	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	141463	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65046	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	59098	4.507	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.200%	
7) Chloroethane-d5	1.571	69	55704	3.993	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	79.800%	
11) 1,1-Dichloroethene-d2	2.111	63	89950	3.424	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.400%	
20) 2-Butanone-d5	3.905	46	82776	51.892	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.780%	
24) Chloroform-d	4.352	84	90507	4.567	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.400%	
26) 1,2-Dichloroethane-d4	5.037	65	44126	5.168	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.400%	
32) Benzene-d6	5.053	84	174656	4.267	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	6.072	67	52814	4.627	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.600%	
41) Toluene-d8	7.317	98	144323	3.800	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.000%	
43) trans-1,3-Dichloroprop...	7.625	79	15225	3.968	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.400%	
46) 2-Hexanone-d5	8.092	63	58682	43.579	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	87.160%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31659	4.390	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50308	4.613	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.200%	
Target Compounds					Qvalue	
25) Chloroform	4.384	83	14464	0.789	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025551.D
Acq On : 14 Apr 2022 17:14
Operator : SY/MD
Sample : N2388-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFE6

Quant Time: Apr 15 07:24:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 15 07:05:00 2022
Response via : Initial Calibration

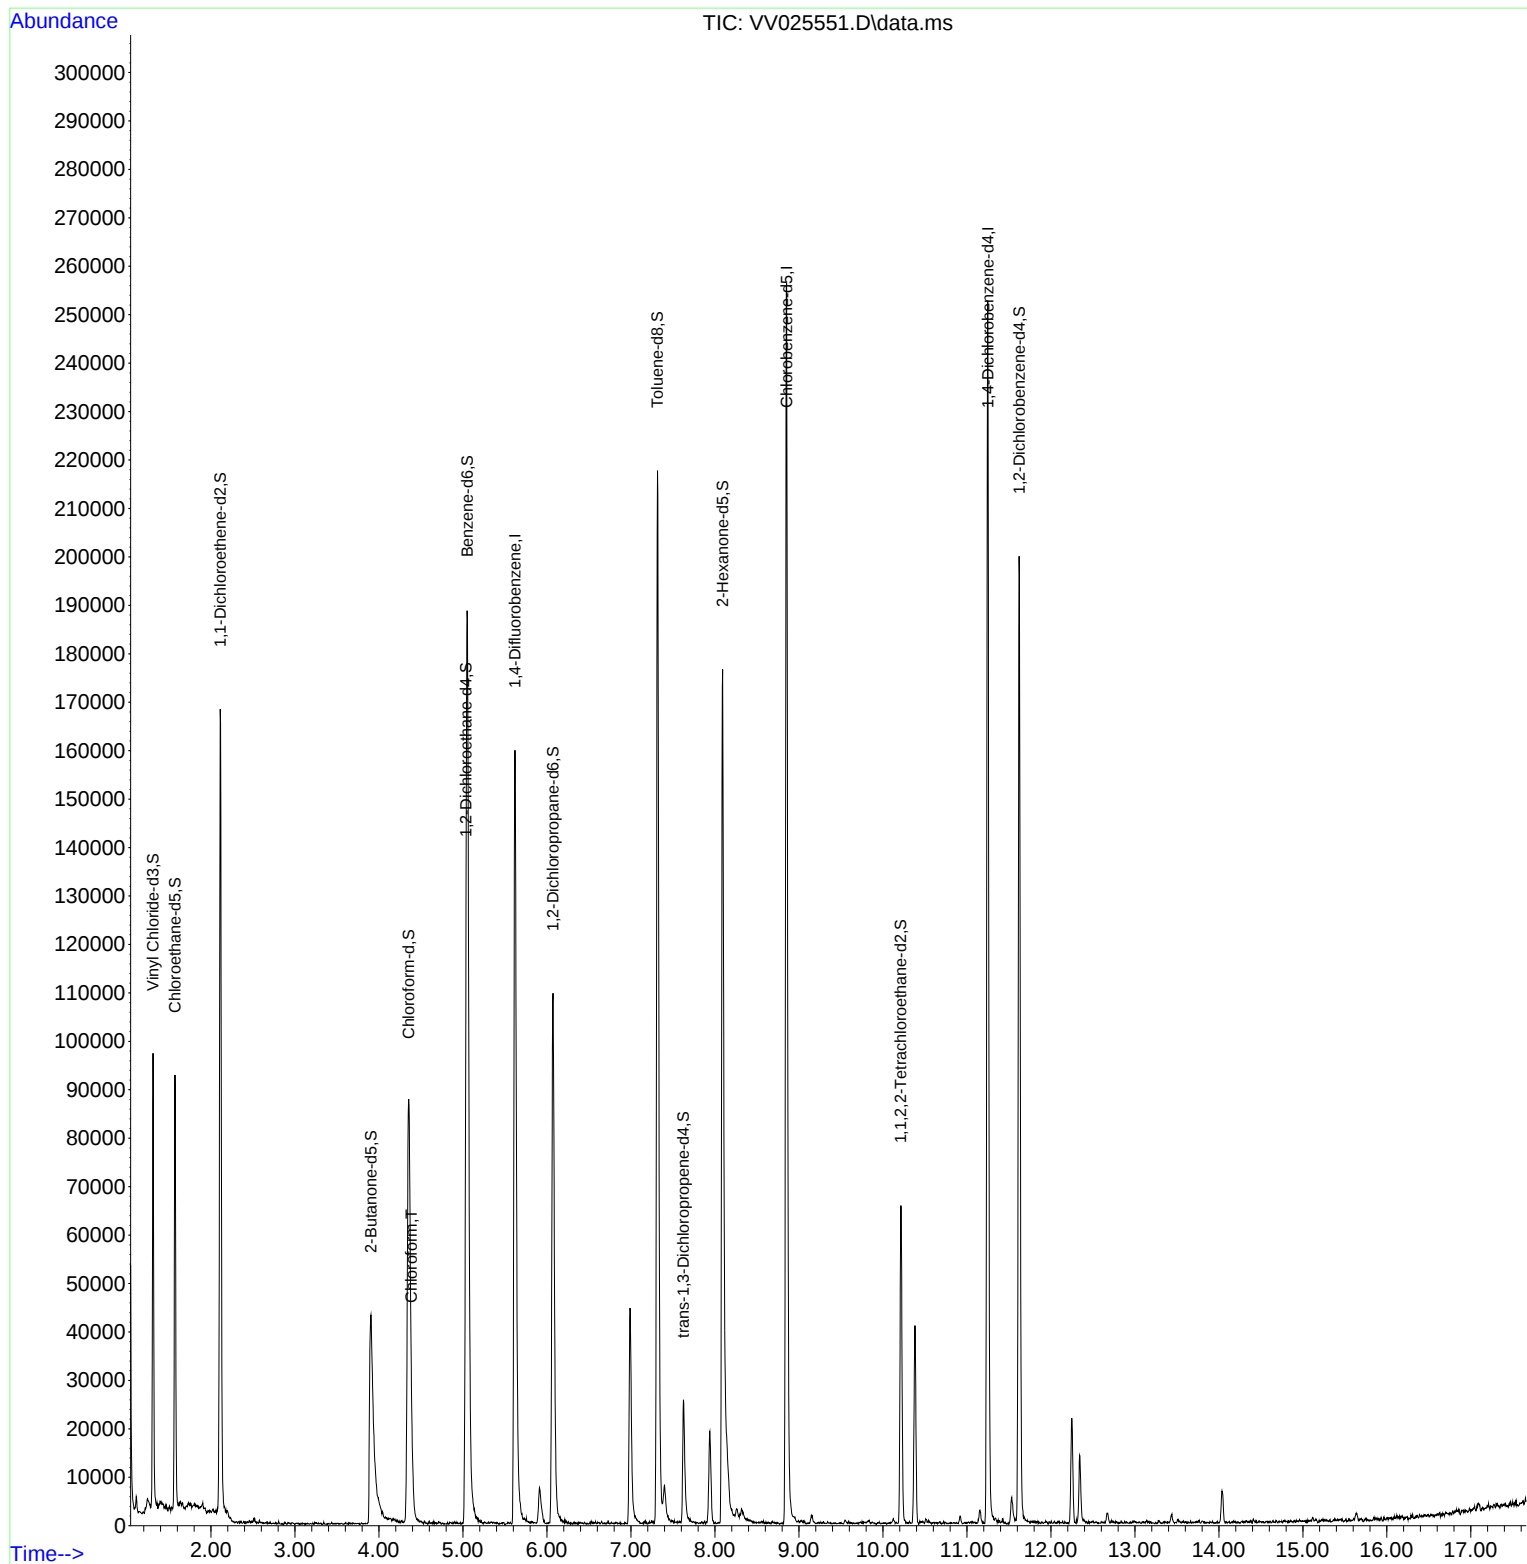

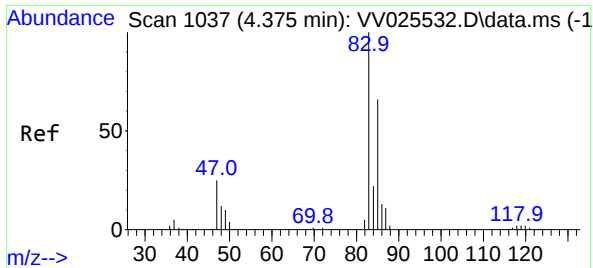

#25
 Chloroform
 Concen: 0.789 ug/L
 RT: 4.384 min Scan# 10
 Delta R.T. 0.010 min
 Lab File: VV025551.D
 Acq: 14 Apr 2022 17:14

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFE6

Tgt Ion: 83 Resp: 14464
 Ion Ratio Lower Upper
 83 100
 85 66.4 43.5 80.7

