

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
 Data File : VV025534.D
 Acq On : 14 Apr 2022 10:36
 Operator : SY/MD
 Sample : N2357-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	93	rBV	114904	117580	20.28%	2.397%
2	1.571	157	165	174	rBV	108308	121395	20.94%	2.475%
3	2.111	321	333	358	rVB	212892	316080	54.52%	6.444%
4	2.513	445	458	473	rBV5	3942	7147	1.23%	0.146%
5	3.895	879	888	919	rBV	40855	142960	24.66%	2.914%
6	4.349	1010	1029	1060	rBV	103431	262966	45.36%	5.361%
7	5.047	1228	1246	1270	rBV2	234207	579775	100.00%	11.819%
8	5.616	1410	1423	1451	rBV	204040	421917	72.77%	8.601%
9	5.915	1506	1516	1534	rBV7	6446	15766	2.72%	0.321%
10	6.069	1550	1564	1585	rBV	130083	273162	47.12%	5.569%
11	6.985	1840	1849	1872	rBV	54459	104992	18.11%	2.140%
12	7.313	1940	1951	1972	rBV	284043	500367	86.30%	10.200%
13	7.625	2038	2048	2067	rBV2	30372	55943	9.65%	1.140%
14	8.088	2182	2192	2226	rBV	185803	377534	65.12%	7.696%
15	8.850	2417	2429	2450	rBV	327863	537136	92.65%	10.950%
16	10.214	2842	2853	2868	rBV	78011	123198	21.25%	2.511%
17	10.381	2895	2905	2915	rVB2	5131	8475	1.46%	0.173%
18	11.246	3162	3174	3197	rBV	336974	518888	89.50%	10.578%
19	11.622	3280	3291	3310	rBV	249869	394287	68.01%	8.038%
20	12.249	3473	3486	3497	rVB	7940	12586	2.17%	0.257%
21	14.040	4034	4043	4052	rVB2	8818	13237	2.28%	0.270%


Sum of corrected areas: 4905391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025534.D
Acq On : 14 Apr 2022 10:36
Operator : SY/MD
Sample : N2357-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

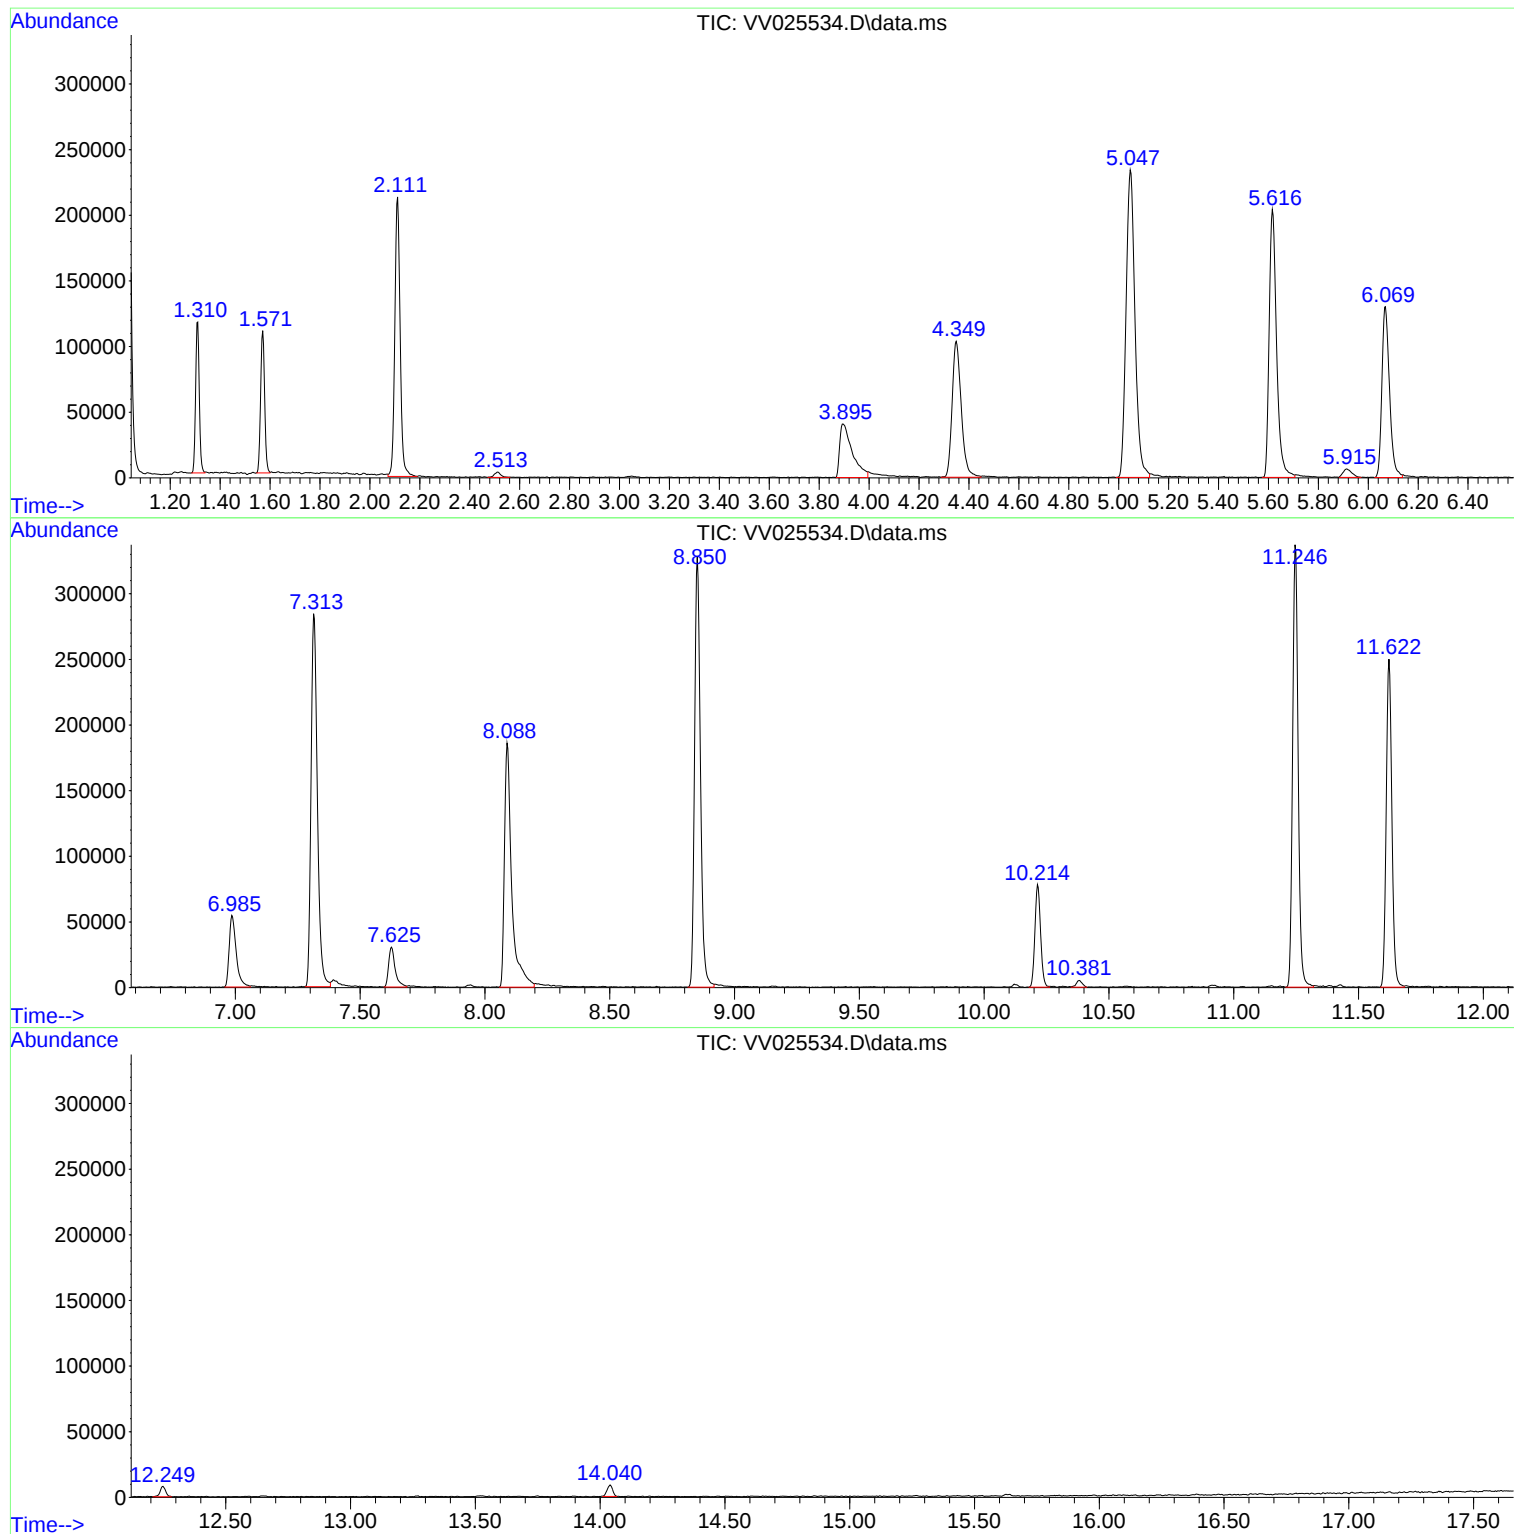

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025534.D
Acq On : 14 Apr 2022 10:36
Operator : SY/MD
Sample : N2357-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025534.D
Acq On : 14 Apr 2022 10:36
Operator : SY/MD
Sample : N2357-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc