

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
 Data File : VV025547.D
 Acq On : 14 Apr 2022 15:40
 Operator : SY/MD
 Sample : N2356-19DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDT7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	100	rVB	92482	92335	19.84%	2.152%
2	1.571	157	165	179	rBV	85410	100131	21.52%	2.333%
3	2.114	323	334	354	rVB	158252	236552	50.83%	5.512%
4	3.912	878	893	927	rBV2	59257	207035	44.49%	4.824%
5	4.352	1011	1030	1055	rBV	83636	211162	45.38%	4.921%
6	5.053	1230	1248	1272	rBV2	182240	457328	98.28%	10.657%
7	5.619	1413	1424	1448	rBV	148101	304622	65.46%	7.098%
8	5.915	1503	1516	1551	rBV	229573	465342	100.00%	10.844%
9	6.072	1551	1565	1585	rBV2	104405	217267	46.69%	5.063%
10	6.992	1839	1851	1874	rBV2	41229	80887	17.38%	1.885%
11	7.317	1940	1952	1972	rBV	210963	371130	79.75%	8.648%
12	7.625	2039	2048	2064	rBV	22798	42291	9.09%	0.985%
13	7.940	2128	2146	2156	rBV3	5107	9228	1.98%	0.215%
14	8.091	2183	2193	2232	rBV	155434	327070	70.29%	7.622%
15	8.854	2417	2430	2450	rBV	235554	390340	83.88%	9.096%
16	10.217	2843	2854	2872	rBV	64819	101683	21.85%	2.369%
17	10.384	2895	2906	2918	rVB2	8604	13869	2.98%	0.323%
18	11.249	3164	3175	3192	rBV	227049	354771	76.24%	8.267%
19	11.622	3280	3291	3312	rBV	181331	288805	62.06%	6.730%
20	12.249	3476	3486	3496	rBV2	7763	12840	2.76%	0.299%
21	14.040	4033	4043	4053	rVB2	4465	6690	1.44%	0.156%




Sum of corrected areas: 4291378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025547.D
Acq On : 14 Apr 2022 15:40
Operator : SY/MD
Sample : N2356-19DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

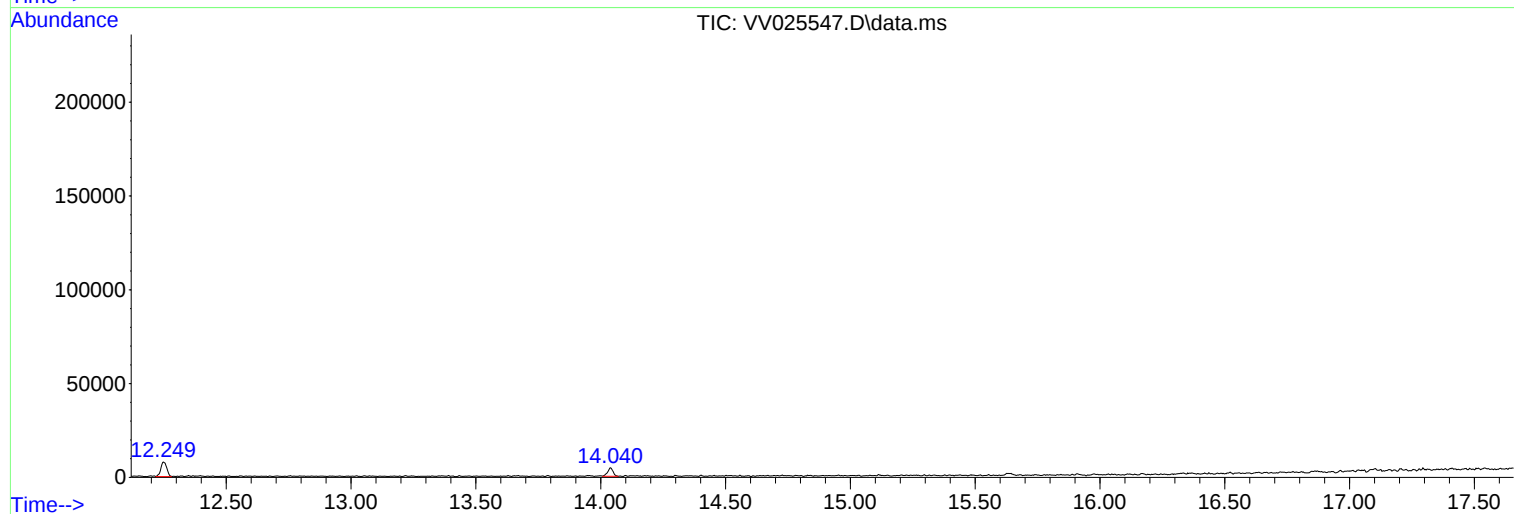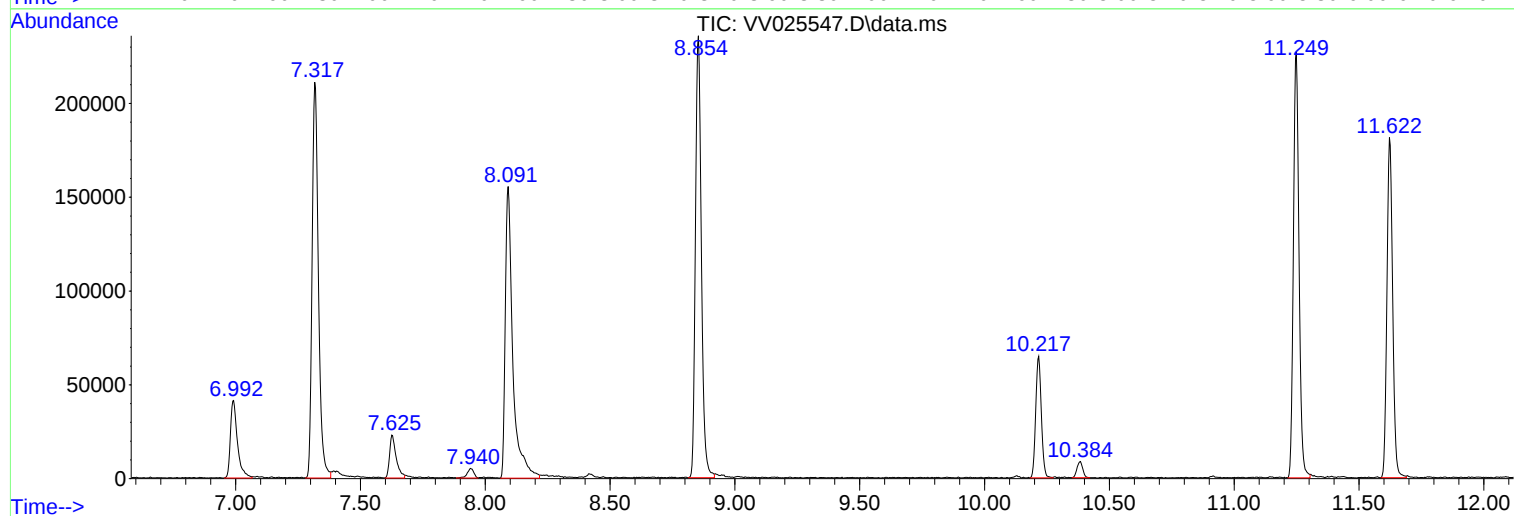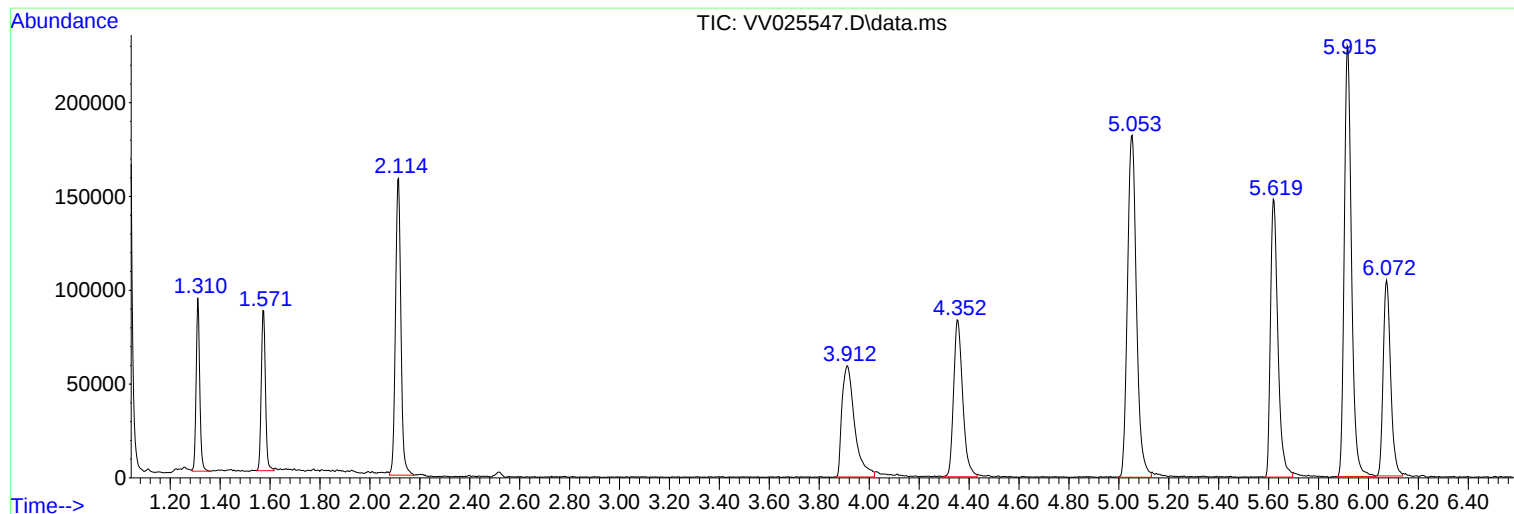

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025547.D
Acq On : 14 Apr 2022 15:40
Operator : SY/MD
Sample : N2356-19DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025547.D
Acq On : 14 Apr 2022 15:40
Operator : SY/MD
Sample : N2356-19DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc