
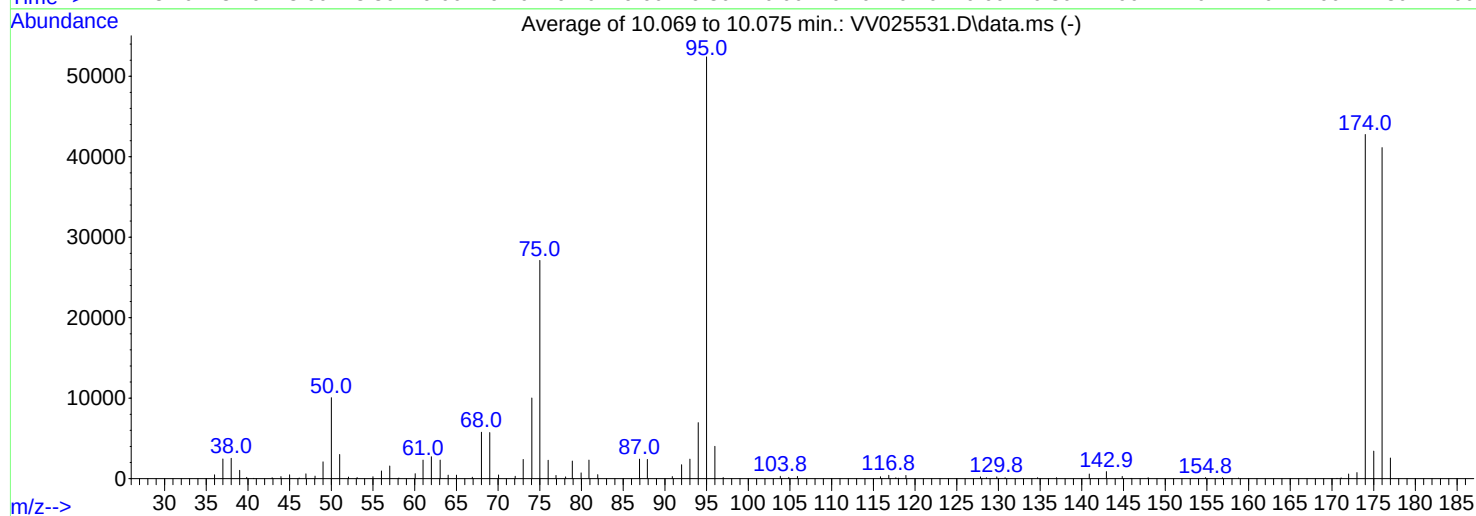


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041422\
Data File : VV025531.D
Acq On : 14 Apr 2022 08:52
Operator : SY/MD
Sample : BFB302
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB302

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 20 02:46:45 2022

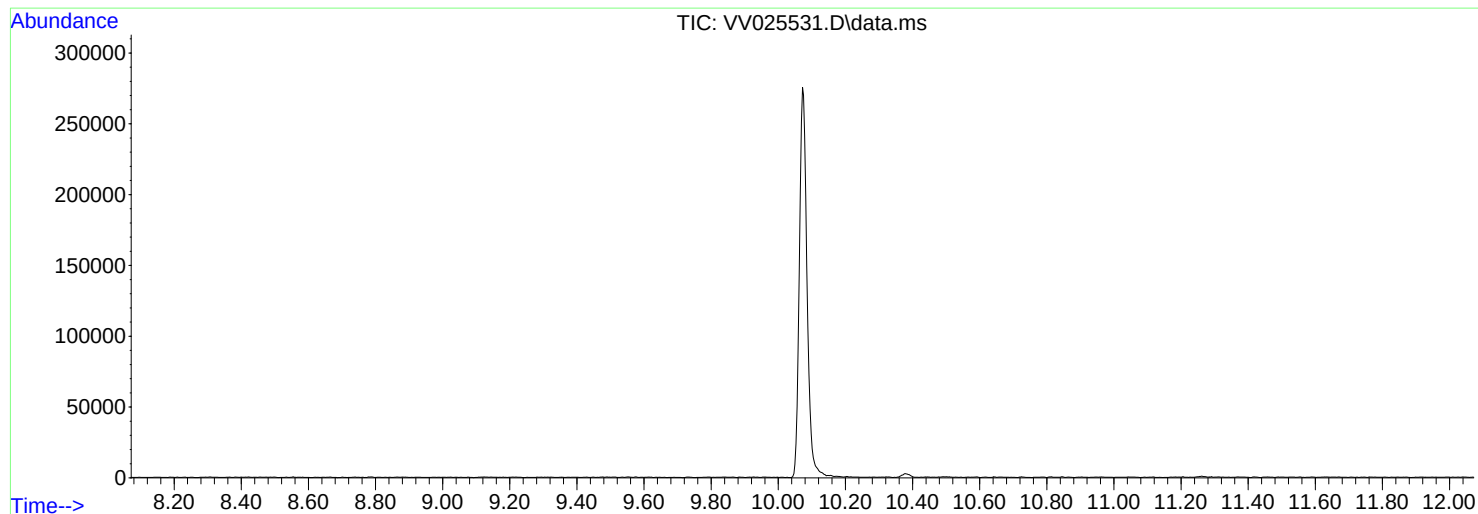

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	10055	PASS
75	95	30	80	51.7	27115	PASS
95	95	100	100	100.0	52411	PASS
96	95	5	9	7.6	4008	PASS
173	174	0.00	2	1.8	751	PASS
174	95	50	120	81.6	42773	PASS
175	174	5	9	8.0	3430	PASS
176	174	95	105	96.2	41133	PASS
177	176	5	10	6.2	2569	PASS

m/z	Abundance
44.00	264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
36.00	488.0
37.00	2559.0
38.00	2518.0
39.00	986.0
39.80	188.0
42.90	105.0
43.90	599.0
45.00	443.0
46.10	119.0
47.00	688.0
48.10	278.0
49.00	2128.0
50.00	9627.0
51.00	2874.0
52.10	172.0
53.10	155.0
55.00	255.0
56.00	973.0
57.00	1536.0
58.10	110.0
60.10	634.0
61.00	2139.0
62.00	2665.0
63.00	2310.0
64.00	472.0
65.00	390.0
66.90	162.0
68.00	5712.0
69.00	5503.0
70.00	404.0
72.10	309.0
73.00	2470.0
74.00	9476.0
75.00	25456.0
76.00	2120.0
76.90	354.0
78.10	203.0
78.90	2004.0
80.00	674.0
80.90	2239.0
82.00	488.0
87.00	2374.0
87.90	2374.0
90.90	245.0
92.00	1601.0
93.00	2252.0
94.00	6785.0
95.00	49816.0
96.00	3853.0
97.00	152.0
103.90	294.0
104.90	155.0
106.00	278.0
115.90	212.0
116.90	423.0
117.70	163.0
118.90	448.0
127.90	183.0
128.60	122.0
129.80	187.0
130.70	107.0
134.80	106.0
137.00	144.0
140.90	509.0
142.90	802.0
144.80	195.0
147.90	107.0
154.90	111.0
156.90	126.0
158.80	116.0
172.00	531.0
173.00	643.0
174.00	39664.0
175.00	3153.0
176.00	38024.0
177.00	2338.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
36.00	497.0
37.00	2515.0
38.00	2622.0
39.00	1036.0
39.90	166.0
42.90	127.0
43.90	526.0
45.00	471.0
46.20	108.0
46.90	634.0
48.00	301.0
49.00	2153.0
50.00	10430.0
51.00	3109.0
52.10	203.0
53.10	159.0
55.00	258.0
56.00	957.0
57.00	1573.0
58.10	109.0
60.10	668.0
61.00	2295.0
62.00	2834.0
63.00	2369.0
64.00	471.0
65.00	440.0
66.90	187.0
68.00	6014.0
69.00	5933.0
70.10	466.0
72.10	313.0
73.00	2462.0
74.10	10425.0
75.00	28112.0
76.00	2351.0
77.00	394.0
78.10	226.0
78.90	2269.0
80.00	734.0
80.90	2377.0
81.90	510.0
87.00	2549.0
87.90	2472.0
90.90	264.0
92.00	1814.0
93.00	2536.0
94.00	7252.0
95.00	54376.0
96.00	4210.0
97.00	171.0
103.80	292.0
104.80	166.0
105.90	286.0
115.90	240.0
116.80	424.0
117.70	169.0
118.90	430.0
127.80	221.0
128.60	123.0
129.80	213.0
130.80	123.0
134.70	123.0
137.00	126.0
140.90	601.0
142.90	885.0
144.80	304.0
145.90	102.0
148.00	118.0
154.90	149.0
156.80	125.0
158.80	101.0
170.60	105.0
171.10	153.0
172.00	618.0
173.00	783.0
174.00	44400.0
175.00	3563.0
176.00	42632.0
177.00	2650.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
36.00	464.0
37.00	2277.0
38.00	2453.0
39.00	1069.0
39.90	149.0
40.70	112.0
42.90	121.0
44.00	458.0
45.00	501.0
46.90	475.0
48.00	369.0
49.00	1989.0
50.00	10109.0
51.00	3036.0
52.00	235.0
53.10	123.0
55.00	209.0
56.00	925.0
57.00	1606.0
60.00	556.0
61.00	2463.0
62.00	2678.0
63.10	2239.0
64.00	387.0
65.00	489.0
66.90	208.0
68.00	5585.0
69.00	5749.0
70.10	475.0
72.00	278.0
73.00	2258.0
74.00	10155.0
75.00	27776.0
76.00	2404.0
77.00	433.0
78.10	248.0
78.90	2291.0
79.90	756.0
80.90	2307.0
81.90	509.0
86.90	2344.0
87.90	2333.0
90.90	251.0
92.00	1760.0
93.00	2516.0
94.00	6854.0
95.00	53040.0
96.00	3961.0
97.00	120.0
103.80	299.0
104.80	149.0
105.80	277.0
115.80	286.0
116.90	440.0
118.00	182.0
118.90	336.0
127.80	225.0
128.50	115.0
129.80	243.0
130.90	142.0
134.60	104.0
136.90	107.0
140.90	626.0
143.00	931.0
144.90	324.0
148.00	130.0
154.80	173.0
156.80	131.0
171.10	173.0
172.00	613.0
173.00	826.0
174.00	44256.0
175.00	3575.0
176.00	42744.0
177.00	2720.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302