

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
 Data File : VV025560.D
 Acq On : 15 Apr 2022 12:03
 Operator : SY/MD
 Sample : VV0415WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK344

Quant Time: Apr 16 02:41:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 16 02:38:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	156321	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150680	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	68240	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	54125	3.724	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.400%
7) Chloroethane-d5	1.574	69	52502	3.396	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.000%
11) 1,1-Dichloroethene-d2	2.111	63	91864	3.155	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.200%
20) 2-Butanone-d5	3.902	46	89316	50.523	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.040%
24) Chloroform-d	4.349	84	97666	4.447	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.034	65	46204	4.883	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.600%
32) Benzene-d6	5.047	84	187734	4.306	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
36) 1,2-Dichloropropane-d6	6.066	67	56617	4.657	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.313	98	154876	3.828	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.600%
43) trans-1,3-Dichloroprop...	7.625	79	16525	4.044	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.800%
46) 2-Hexanone-d5	8.088	63	63806	44.485	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.980%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32896	4.282	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	51486	4.500	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.000%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	6525	0.496	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025560.D
Acq On : 15 Apr 2022 12:03
Operator : SY/MD
Sample : VV0415WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK344


Quant Time: Apr 16 02:41:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 16 02:38:36 2022
Response via : Initial Calibration

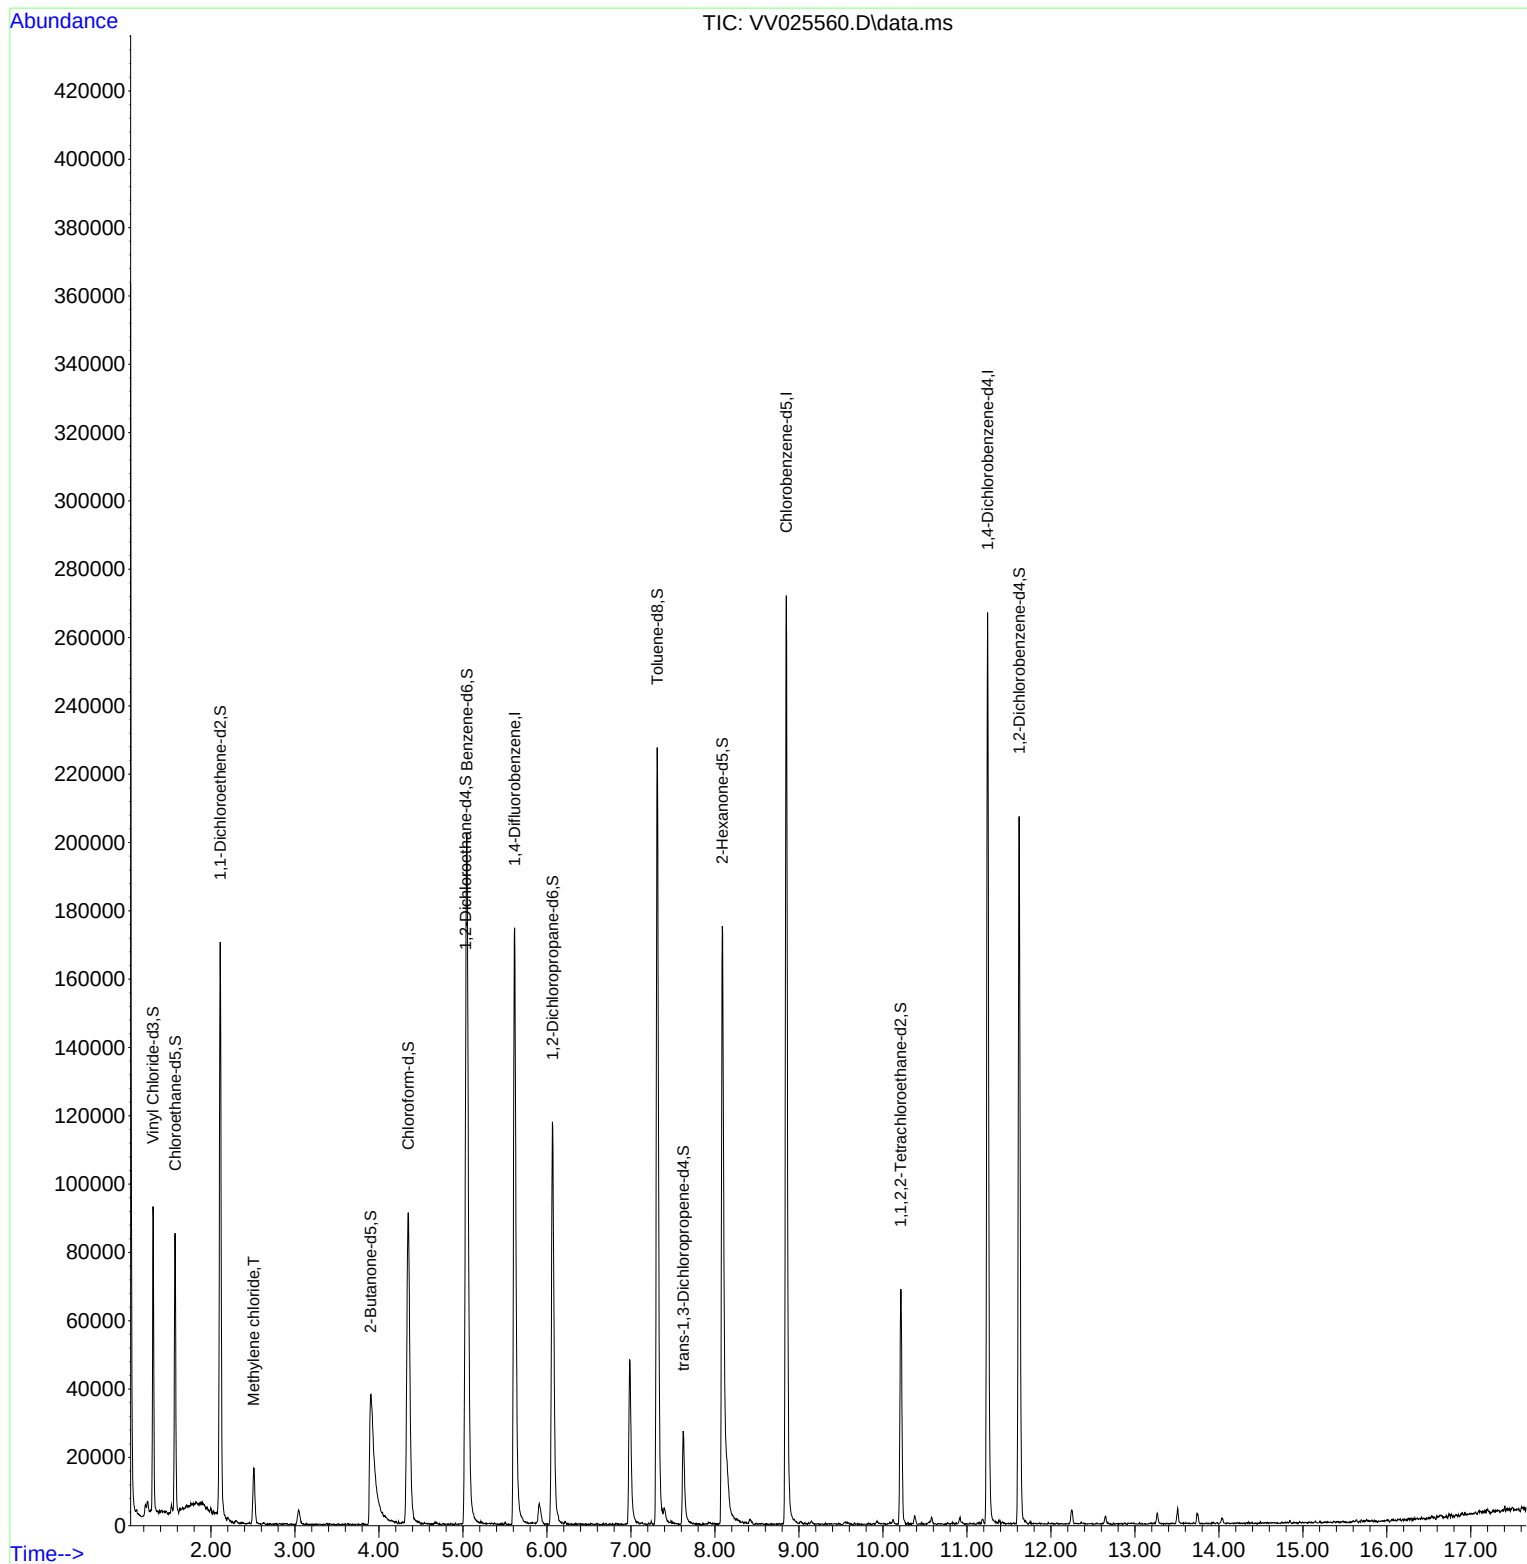

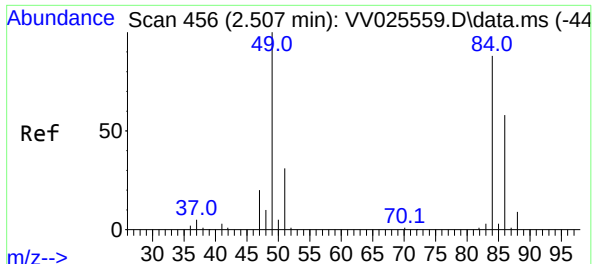

#16
Methylene chloride
Concen: 0.496 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025560.D
Acq: 15 Apr 2022 12:03

Instrument :
MSVOA_V
ClientSampleId :
VBLK344

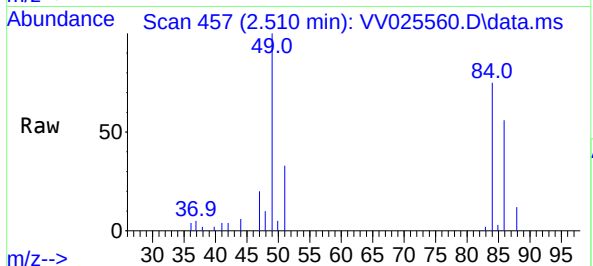

Tgt Ion: 84 Resp: 6525

Ion	Ratio	Lower	Upper
84	100		
86	75.3	45.9	85.3
49	134.1	76.6	142.3

