

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041522\
 Data File : VW025561.D
 Acq On : 15 Apr 2022 12:36
 Operator : SY/MD
 Sample : N2373-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 16 02:41:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 16 02:38:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	185262	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	182296	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	84724	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	65097	3.779	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.600%
7) Chloroethane-d5	1.571	69	64326	3.511	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.200%
11) 1,1-Dichloroethene-d2	2.111	63	105943	3.070	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.400%
20) 2-Butanone-d5	3.899	46	98420	46.976	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.960%
24) Chloroform-d	4.349	84	110167	4.233	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	5.034	65	51287	4.573	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
32) Benzene-d6	5.047	84	217132	4.117	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.400%
36) 1,2-Dichloropropane-d6	6.066	67	65852	4.477	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.600%
41) Toluene-d8	7.313	98	183575	3.750	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.000%
43) trans-1,3-Dichloroprop...	7.622	79	18238	3.689	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.800%
46) 2-Hexanone-d5	8.088	63	69470	40.034	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.060%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38191	4.109	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	61408	4.323	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.400%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	10281	0.660	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025561.D
Acq On : 15 Apr 2022 12:36
Operator : SY/MD
Sample : N2373-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Apr 16 02:41:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 16 02:38:36 2022
Response via : Initial Calibration

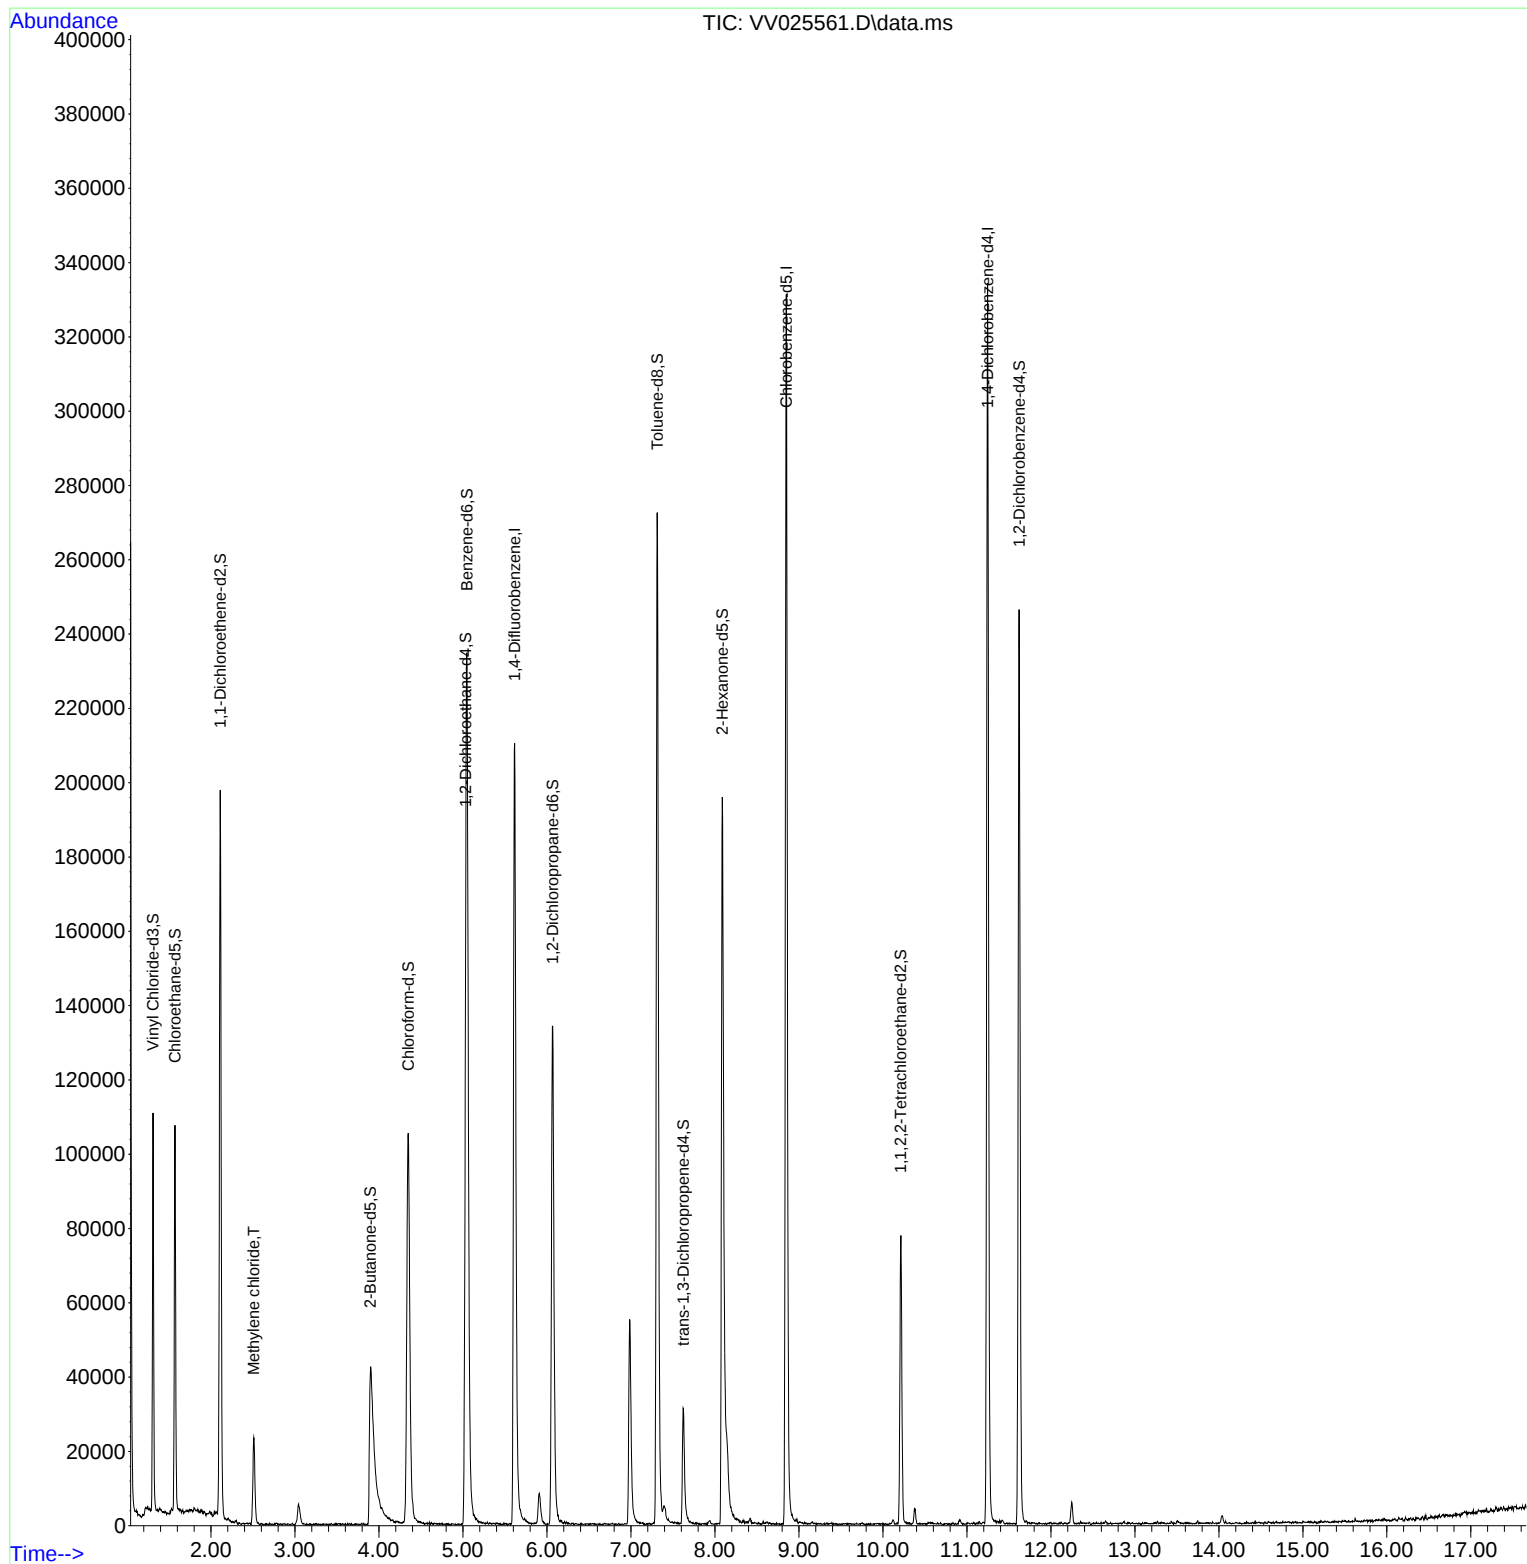

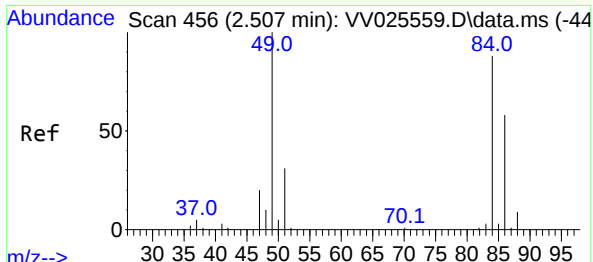

#16
Methylene chloride
Concen: 0.660 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025561.D
Acq: 15 Apr 2022 12:36

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

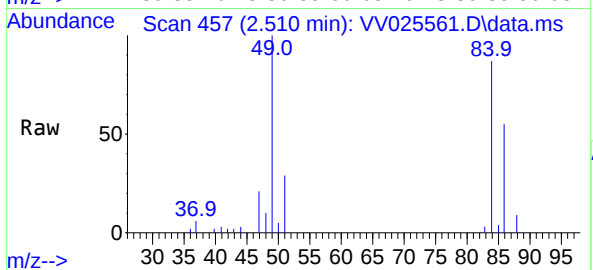

Tgt Ion: 84 Resp: 10281

Ion	Ratio	Lower	Upper
84	100		
86	62.8	45.9	85.3
49	114.4	76.6	142.3

