

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW041522\  
 Data File : VW025563.D  
 Acq On : 15 Apr 2022 13:22  
 Operator : SY/MD  
 Sample : N2388-06  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BFFE9

Quant Time: Apr 16 02:42:16 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR040822WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Apr 16 02:38:36 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min)  |
|-------------------------------|--------|-------|----------|----------|-------|-----------|
| -----                         |        |       |          |          |       |           |
| Internal Standards            |        |       |          |          |       |           |
| 1) 1,4-Difluorobenzene        | 5.619  | 114   | 120850   | 5.000    | ug/L  | 0.00      |
| 28) Chlorobenzene-d5          | 8.854  | 117   | 123676   | 5.000    | ug/L  | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152   | 56436    | 5.000    | ug/L  | 0.00      |
| System Monitoring Compounds   |        |       |          |          |       |           |
| 4) Vinyl Chloride-d3          | 1.310  | 65    | 44347    | 3.947    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 79.000%   |
| 7) Chloroethane-d5            | 1.574  | 69    | 43247    | 3.618    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 72.400%   |
| 11) 1,1-Dichloroethene-d2     | 2.114  | 63    | 68320    | 3.035    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 60.800%   |
| 20) 2-Butanone-d5             | 3.902  | 46    | 66598    | 48.729   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 97.460%   |
| 24) Chloroform-d              | 4.355  | 84    | 76807    | 4.524    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 90.400%   |
| 26) 1,2-Dichloroethane-d4     | 5.037  | 65    | 35428    | 4.843    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 96.800%   |
| 32) Benzene-d6                | 5.053  | 84    | 144205   | 4.030    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 80.600%   |
| 36) 1,2-Dichloropropane-d6    | 6.072  | 67    | 44252    | 4.434    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 88.600%   |
| 41) Toluene-d8                | 7.317  | 98    | 119258   | 3.591    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 71.800%   |
| 43) trans-1,3-Dichloroprop... | 7.628  | 79    | 11549    | 3.443    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 68.800%   |
| 46) 2-Hexanone-d5             | 8.088  | 63    | 42185    | 35.833   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 71.660%   |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84    | 24657    | 3.911    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 78.200%   |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152   | 40963    | 4.329    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 86.600%   |
| Target Compounds              |        |       |          |          |       |           |
| 25) Chloroform                | 4.384  | 83    | 11621    | 0.740    | ug/L  | Qvalue 93 |
| -----                         |        |       |          |          |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV041522\  
Data File : VV025563.D  
Acq On : 15 Apr 2022 13:22  
Operator : SY/MD  
Sample : N2388-06  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFFE9

Quant Time: Apr 16 02:42:16 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR040822WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Apr 16 02:38:36 2022  
Response via : Initial Calibration

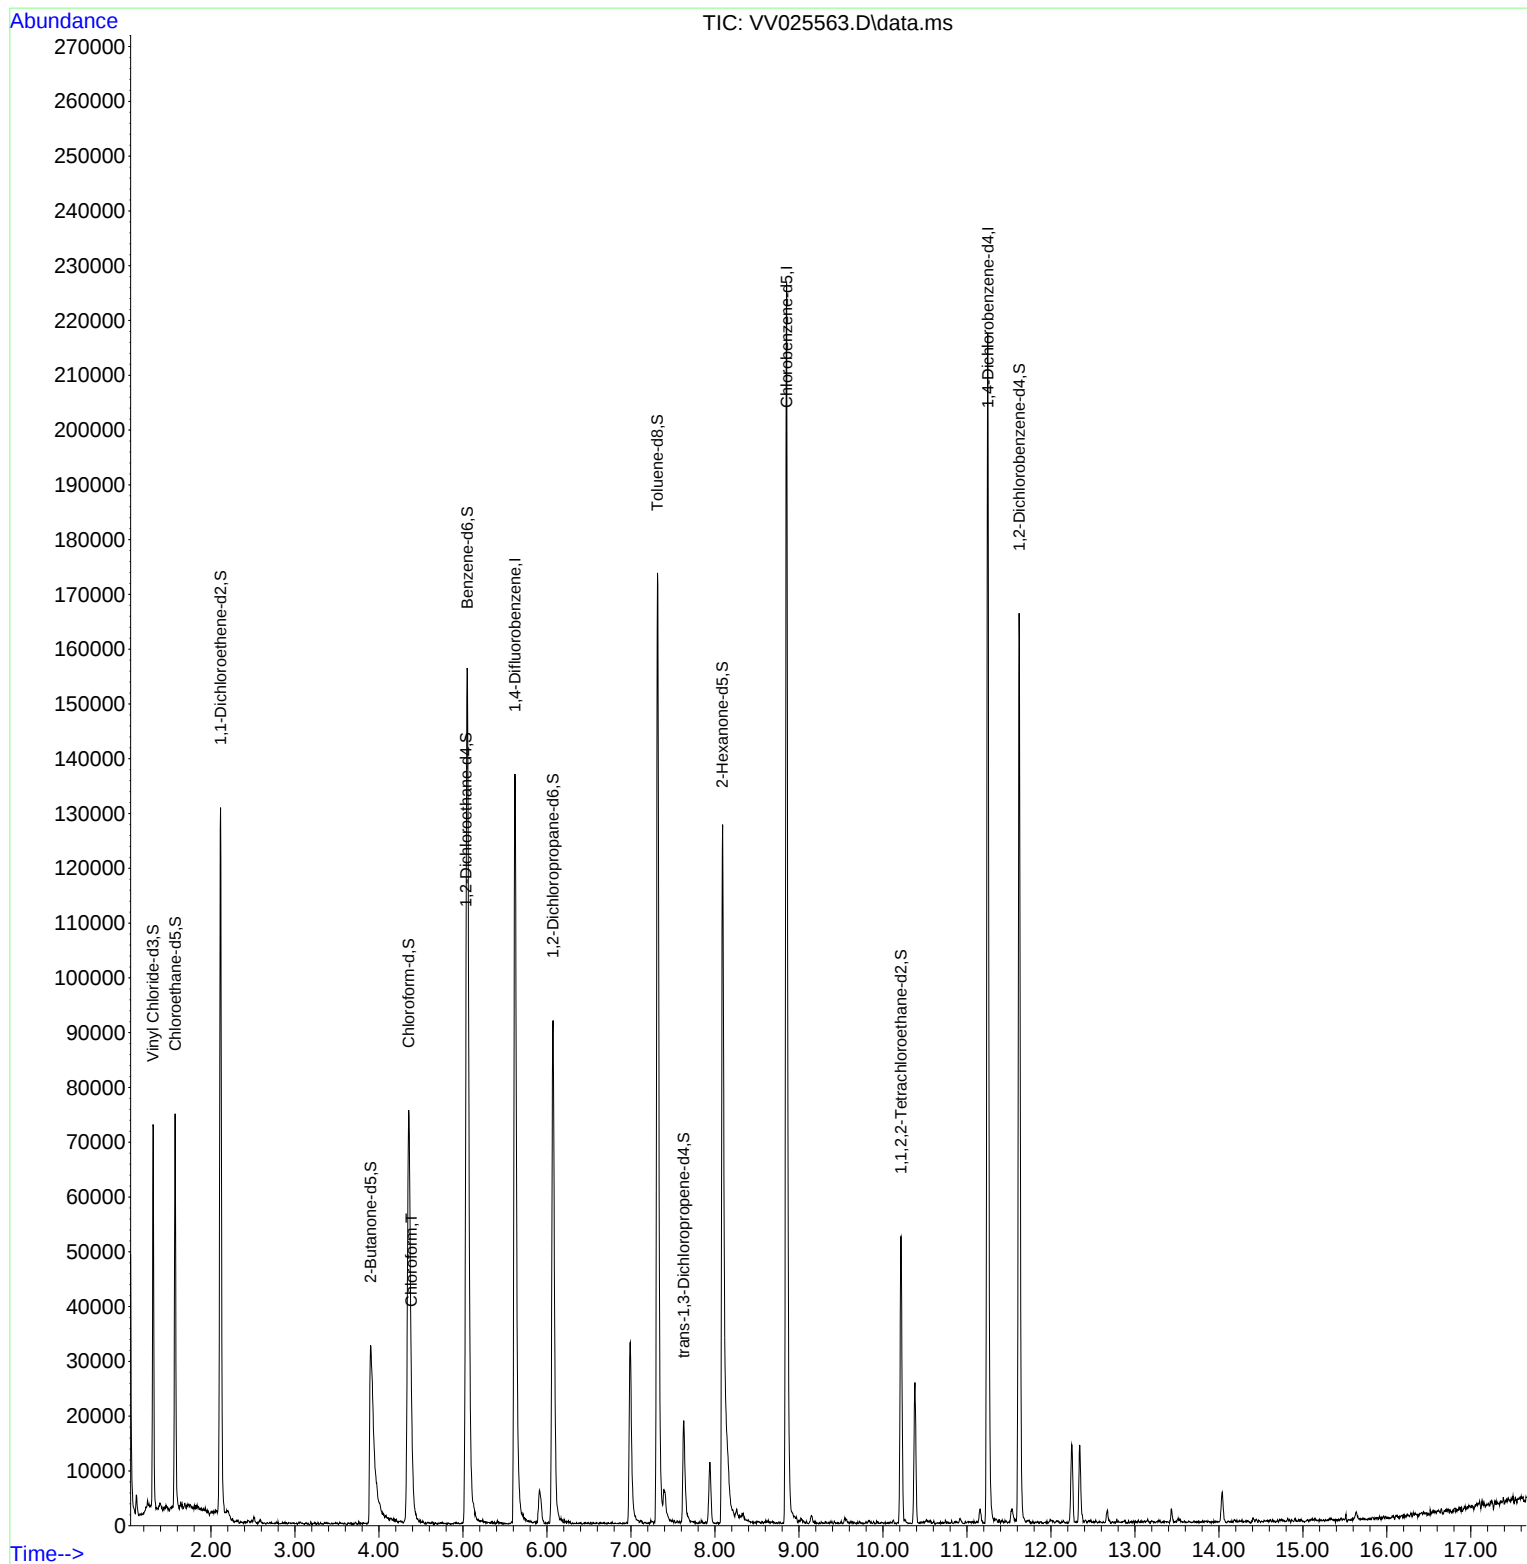

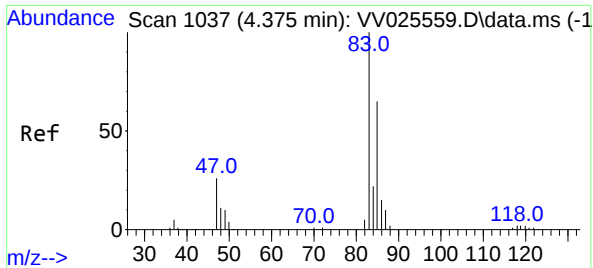

#25  
Chloroform  
Concen: 0.740 ug/L  
RT: 4.384 min Scan# 10  
Delta R.T. 0.010 min  
Lab File: VV025563.D  
Acq: 15 Apr 2022 13:22

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFFE9

Tgt Ion: 83 Resp: 11621  
Ion Ratio Lower Upper  
83 100  
85 67.2 43.5 80.7

