

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041522\
 Data File : VW025575.D
 Acq On : 15 Apr 2022 18:03
 Operator : SY/MD
 Sample : N2384-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Q3

Quant Time: Apr 16 02:44:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 16 02:38:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	116725	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	121518	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55575	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	43345	3.994	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.800%
7) Chloroethane-d5	1.574	69	44477	3.853	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.000%
11) 1,1-Dichloroethene-d2	2.114	63	68809	3.165	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	3.905	46	64084	48.547	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.100%
24) Chloroform-d	4.355	84	74684	4.554	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	5.037	65	35346	5.002	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.000%
32) Benzene-d6	5.053	84	143448	4.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.600%
36) 1,2-Dichloropropane-d6	6.072	67	44238	4.512	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.200%
41) Toluene-d8	7.316	98	115711	3.546	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.000%
43) trans-1,3-Dichloroprop...	7.628	79	11671	3.541	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.800%
46) 2-Hexanone-d5	8.091	63	45318	39.178	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.360%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26203	4.230	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	38803	4.164	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.200%
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	59719	8.003	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025575.D
Acq On : 15 Apr 2022 18:03
Operator : SY/MD
Sample : N2384-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Q3

Quant Time: Apr 16 02:44:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 16 02:38:36 2022
Response via : Initial Calibration

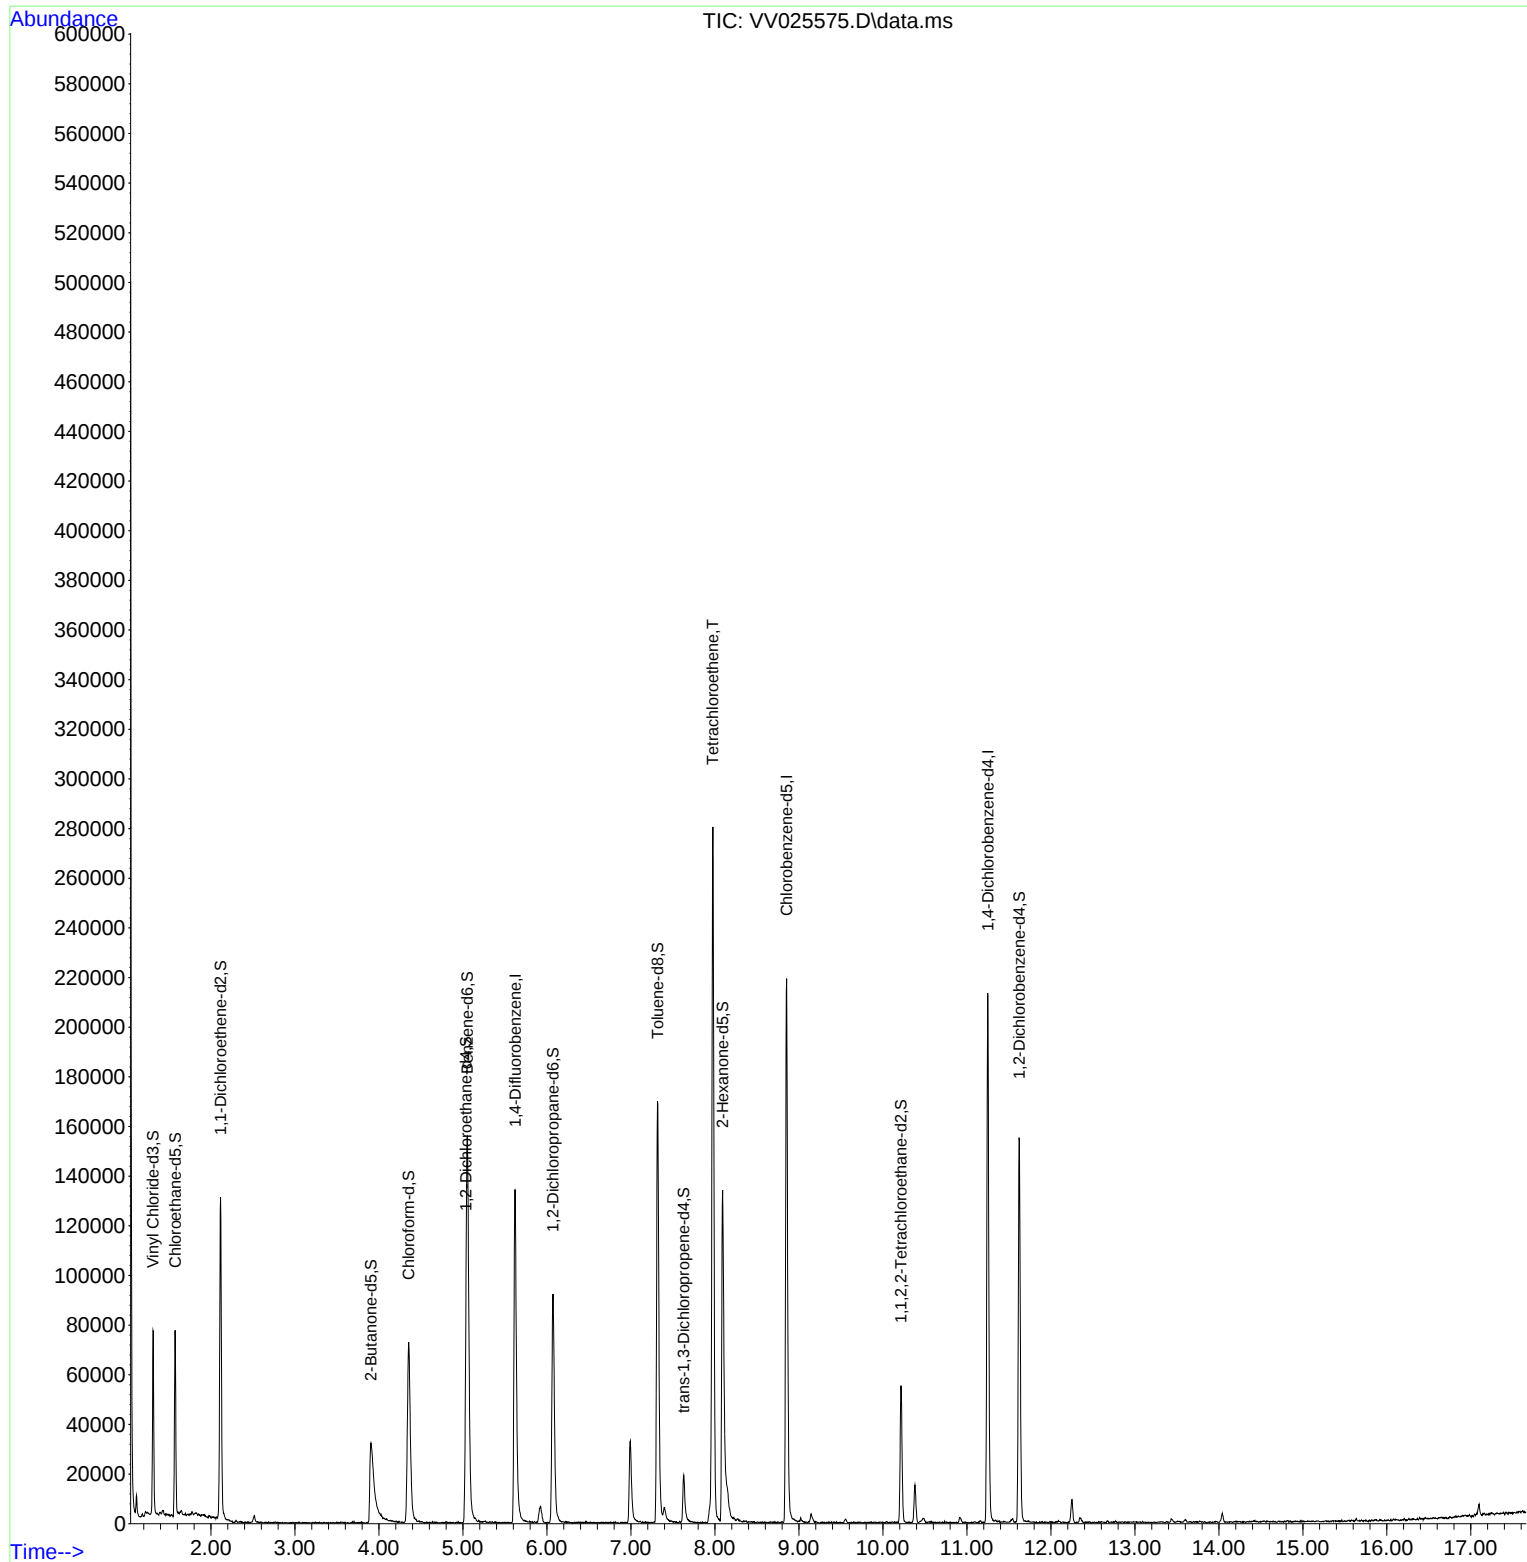

Abundance Scan 2156 (7.973 min): VV025559.D\data.ms (-2

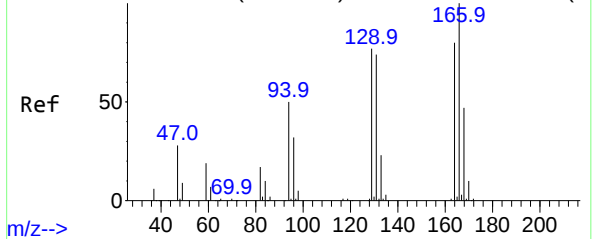

#47

Tetrachloroethene

Concen: 8.003 ug/L

RT: 7.976 min Scan# 21

Delta R.T. 0.003 min

Lab File: VV025575.D

Acq: 15 Apr 2022 18:03


Instrument :

MSVOA_V

ClientSampleId :

EW6Q3

Abundance Scan 2157 (7.976 min): VV025575.D\data.ms

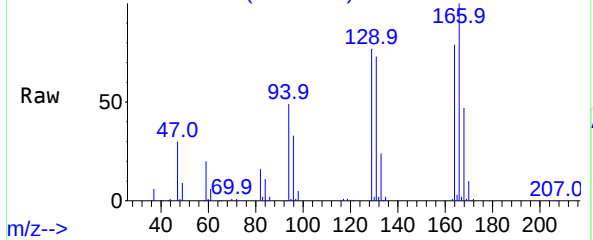

Tgt Ion:164 Resp: 59719

Ion Ratio Lower Upper


164 100

129 98.1 66.8 124.2

131 93.3 66.4 123.4

166 127.4 91.7 170.3

Abundance

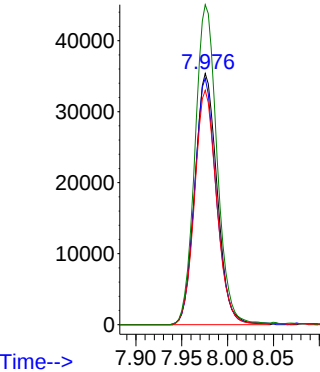

Abundance Scan 2157 (7.976 min): VV025575.D\data.ms (-2

