

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
 Data File : VV025582.D
 Acq On : 15 Apr 2022 21:57
 Operator : SY/MD
 Sample : VV0415WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK345

Quant Time: Apr 16 04:36:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 16 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	137107	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	138160	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60005	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	50148	3.934	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.600%
7) Chloroethane-d5	1.574	69	49401	3.643	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	72.800%
11) 1,1-Dichloroethene-d2	2.114	63	77084	3.019	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.400%
20) 2-Butanone-d5	3.899	46	84408	54.438	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.880%
24) Chloroform-d	4.352	84	91475	4.749	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	5.037	65	43152	5.199	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	5.053	84	174732	4.371	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
36) 1,2-Dichloropropane-d6	6.072	67	54575	4.895	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.000%
41) Toluene-d8	7.317	98	143903	3.879	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.600%
43) trans-1,3-Dichloroprop...	7.625	79	14860	3.966	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.400%
46) 2-Hexanone-d5	8.091	63	59538	45.271	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.540%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32460	4.609	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	48395	4.810	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds						Qvalue
16) Methylene chloride	2.516	84	2741	0.238	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025582.D
Acq On : 15 Apr 2022 21:57
Operator : SY/MD
Sample : VV0415WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK345


Quant Time: Apr 16 04:36:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 16 04:36:16 2022
Response via : Initial Calibration

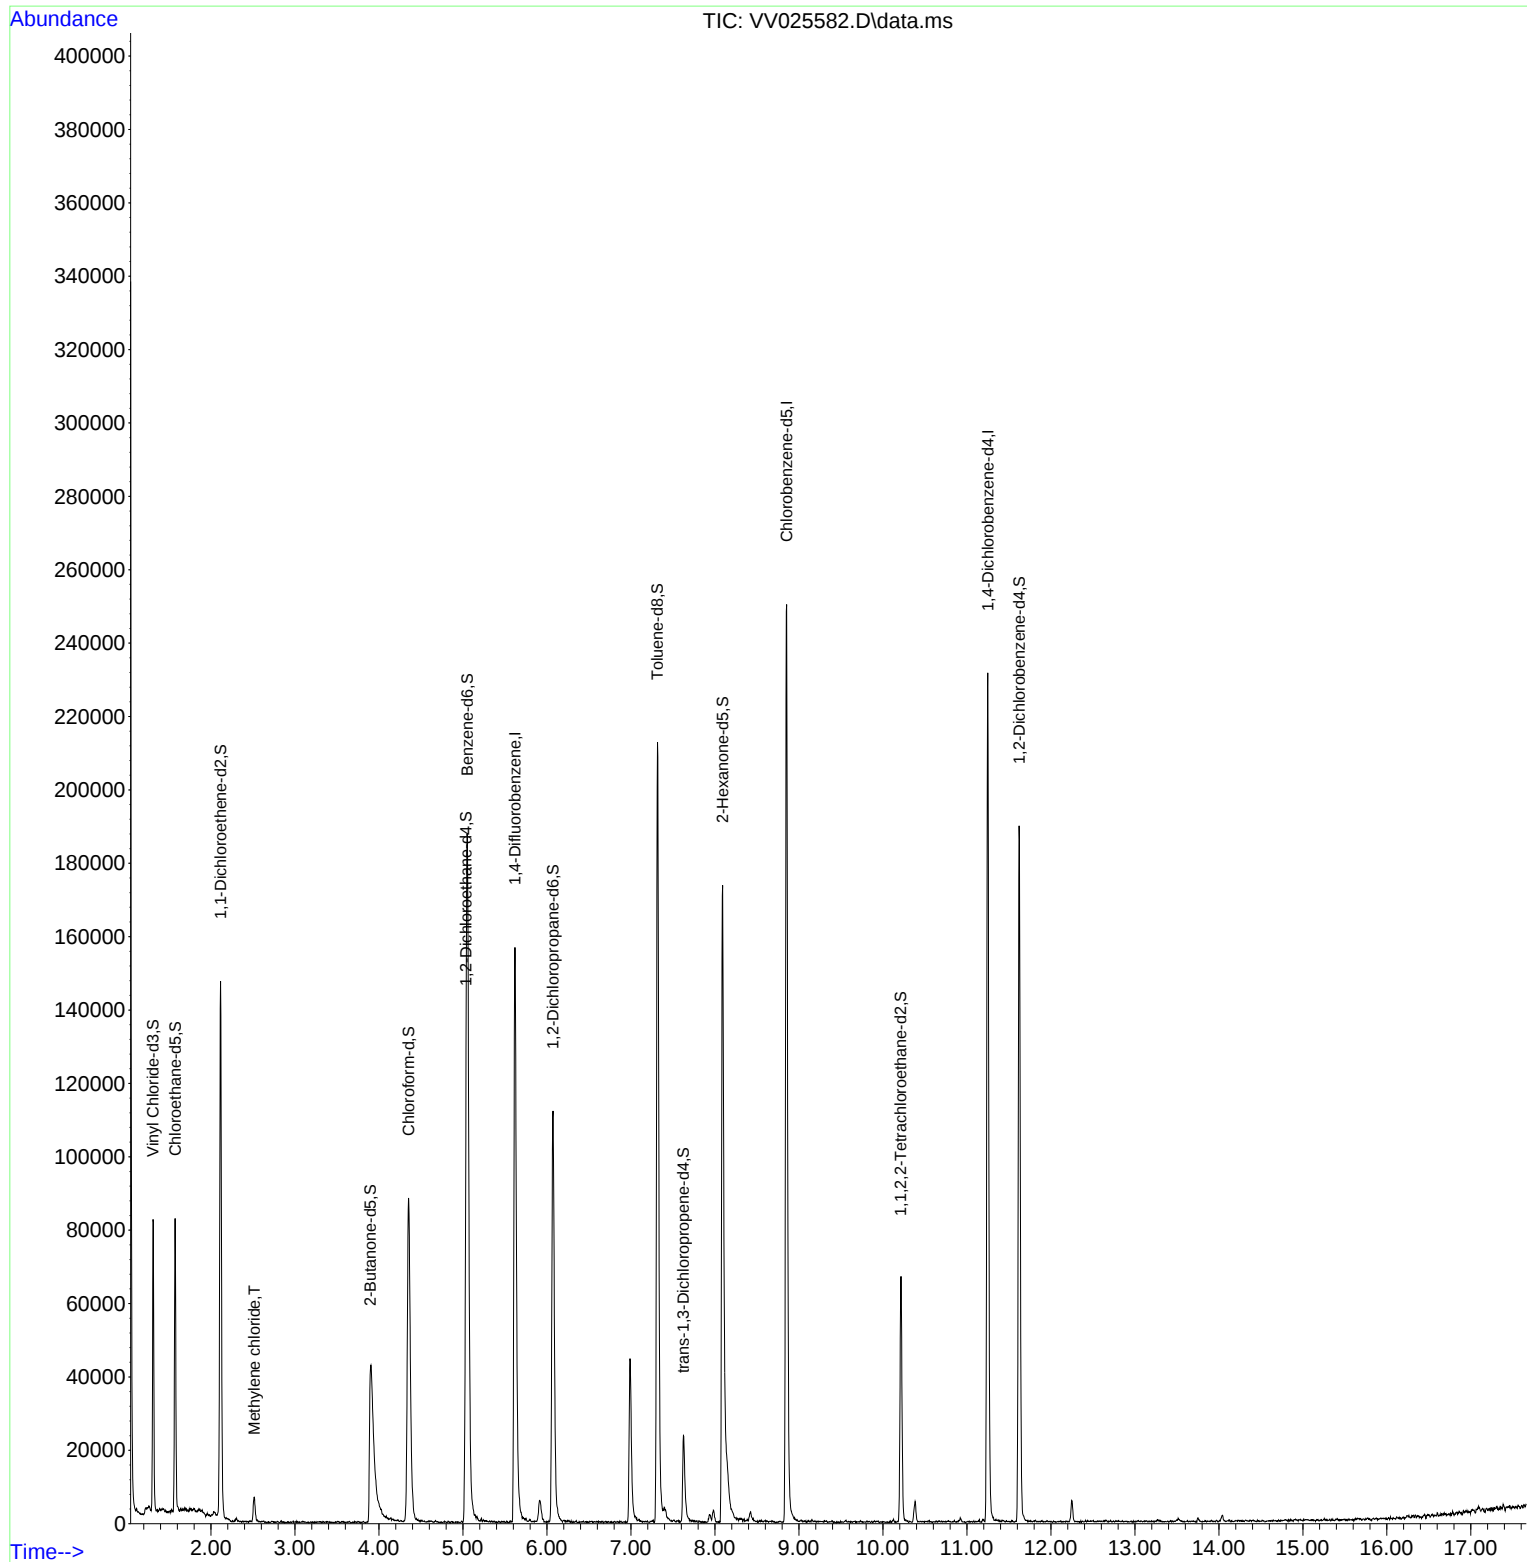

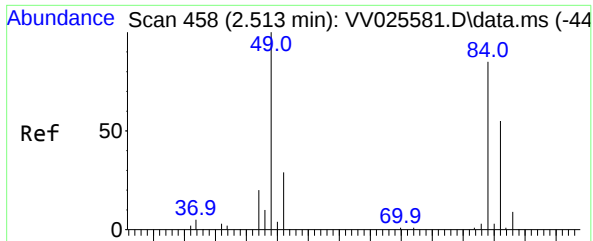

#16
Methylene chloride
Concen: 0.238 ug/L
RT: 2.516 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025582.D
Acq: 15 Apr 2022 21:57

Instrument :
MSVOA_V
ClientSampleId :
VBLK345

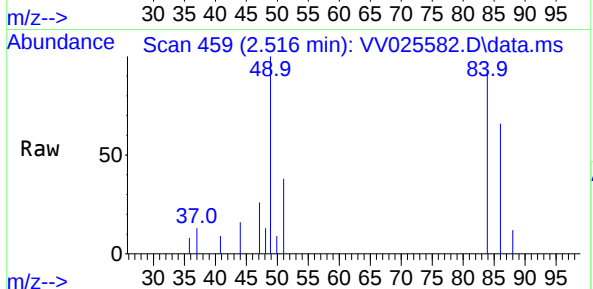

Tgt Ion: 84 Resp: 2741

Ion	Ratio	Lower	Upper
84	100		
86	70.4	45.9	85.3
49	107.3	76.6	142.3

