

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041522\
 Data File : VW025585.D
 Acq On : 15 Apr 2022 23:07
 Operator : SY/MD
 Sample : N2438-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6S1

Quant Time: Apr 16 04:49:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 16 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121686	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125776	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	53626	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	45341	4.008	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.200%
7) Chloroethane-d5	1.571	69	46703	3.880	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.600%
11) 1,1-Dichloroethene-d2	2.111	63	73401	3.239	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.800%
20) 2-Butanone-d5	3.921	46	77371	56.223	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.440%
24) Chloroform-d	4.352	84	83961	4.911	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.037	65	40351	5.478	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%
32) Benzene-d6	5.053	84	152776	4.198	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	6.072	67	48950	4.823	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.400%
41) Toluene-d8	7.316	98	125349	3.712	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.200%
43) trans-1,3-Dichloroprop...	7.625	79	13188	3.866	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.400%
46) 2-Hexanone-d5	8.091	63	56794	47.437	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.880%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32018	4.993	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	43616	4.851	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.976	164	4082	0.529	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025585.D
Acq On : 15 Apr 2022 23:07
Operator : SY/MD
Sample : N2438-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6S1


Quant Time: Apr 16 04:49:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 16 04:36:16 2022
Response via : Initial Calibration

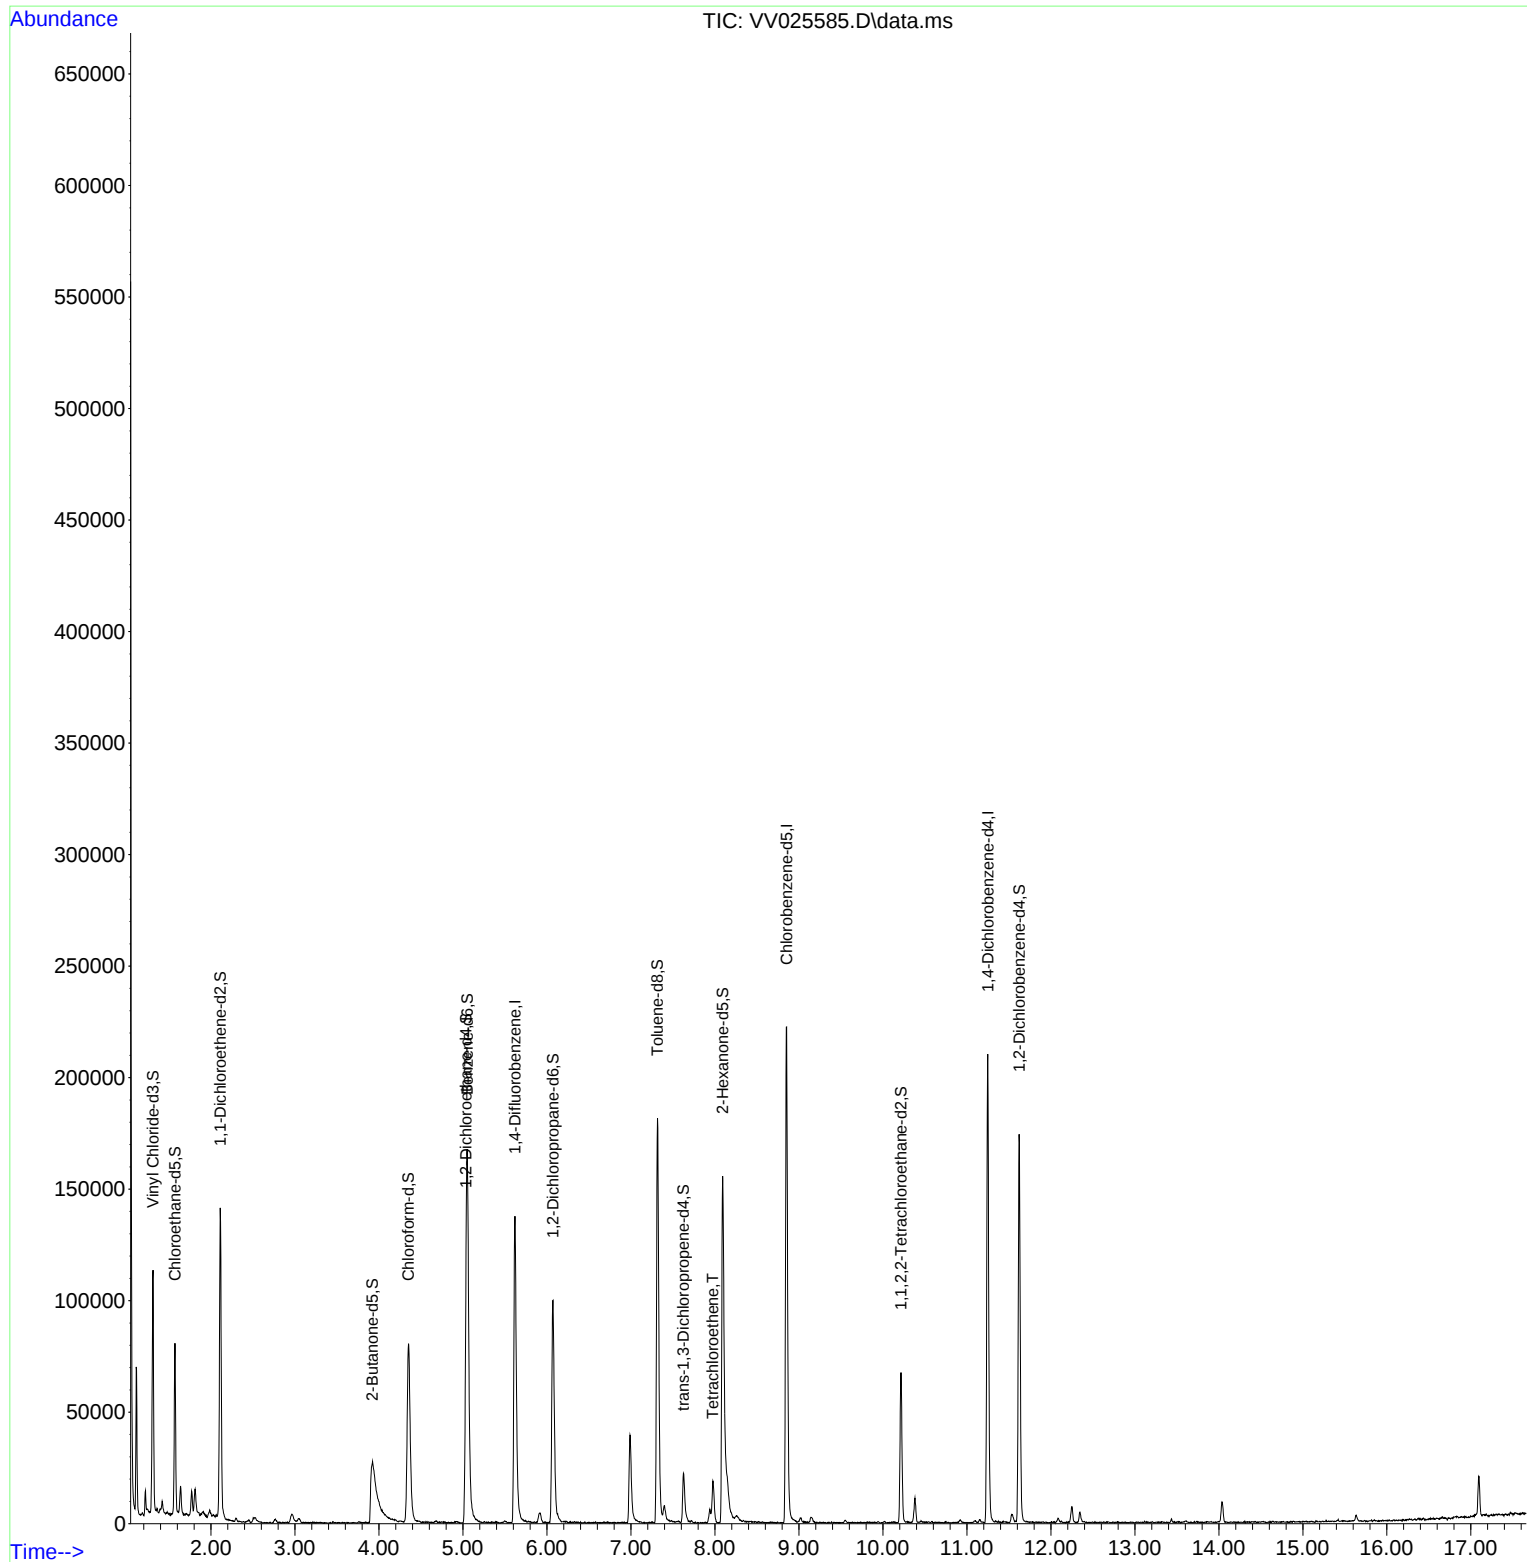

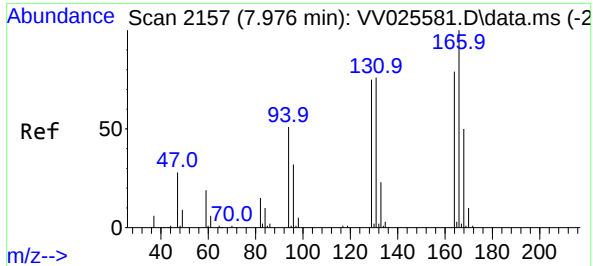

#47
 Tetrachloroethene
 Concen: 0.529 ug/L
 RT: 7.976 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VV025585.D
 Acq: 15 Apr 2022 23:07

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6S1

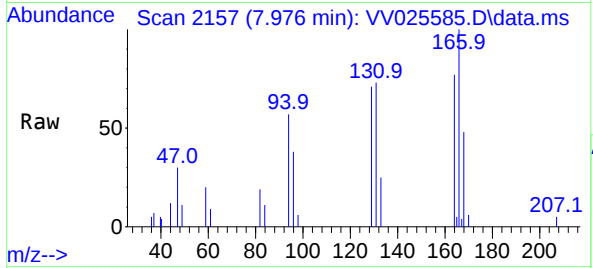

Tgt Ion:164 Resp: 4082

Ion	Ratio	Lower	Upper
164	100		
129	92.5	66.8	124.2
131	95.8	66.4	123.4
166	130.5	91.7	170.3

