

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041522\
 Data File : VW025589.D
 Acq On : 16 Apr 2022 00:41
 Operator : SY/MD
 Sample : N2438-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6S5

Quant Time: Apr 16 04:49:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 16 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	116931	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	119513	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52016	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	42546	3.914	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.200%
7) Chloroethane-d5	1.571	69	44697	3.865	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.200%
11) 1,1-Dichloroethene-d2	2.111	63	67136	3.083	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.600%
20) 2-Butanone-d5	3.895	46	76141	57.579	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.160%
24) Chloroform-d	4.355	84	81650	4.970	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
26) 1,2-Dichloroethane-d4	5.037	65	38259	5.405	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.200%
32) Benzene-d6	5.053	84	148096	4.283	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.072	67	48500	5.029	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.600%
41) Toluene-d8	7.316	98	120038	3.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.800%
43) trans-1,3-Dichloroprop...	7.625	79	12936	3.991	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.088	63	56743	49.878	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.760%
56) 1,1,2,2-Tetrachloroeth...	10.213	84	32990	5.415	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	42714	4.898	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	43328	5.904	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025589.D
Acq On : 16 Apr 2022 00:41
Operator : SY/MD
Sample : N2438-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6S5

Quant Time: Apr 16 04:49:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 16 04:36:16 2022
Response via : Initial Calibration

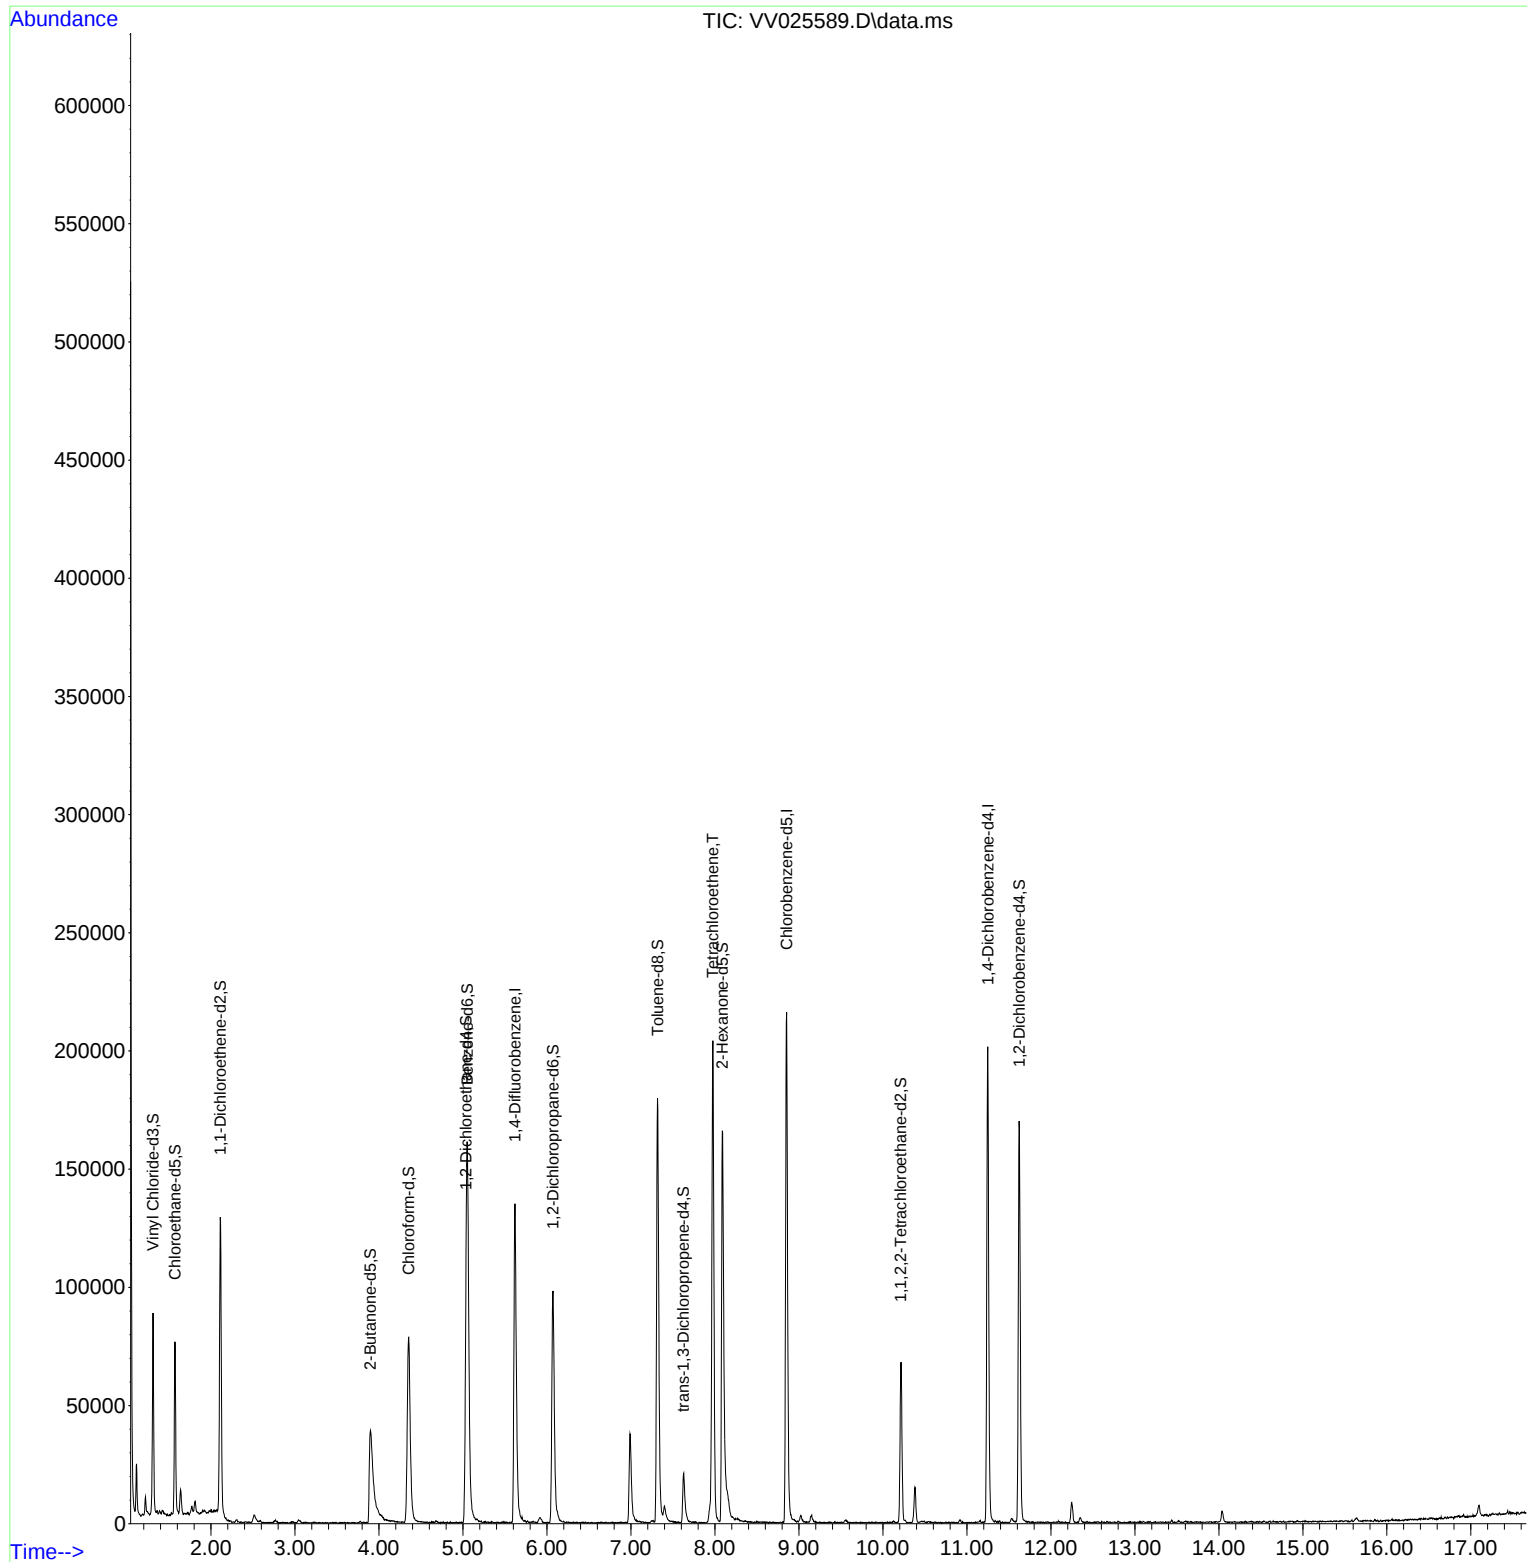

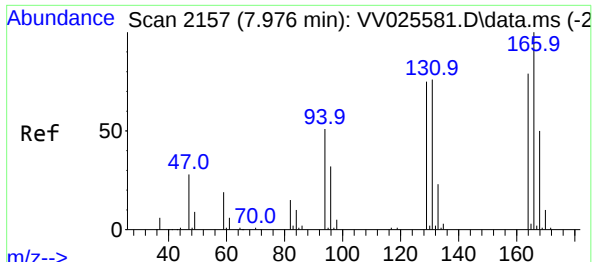

#47
Tetrachloroethene
Concen: 5.904 ug/L
RT: 7.976 min Scan# 21
Delta R.T. -0.000 min
Lab File: VV025589.D
Acq: 16 Apr 2022 00:41

Instrument :
MSVOA_V
ClientSampleId :
EW6S5

Tgt Ion:164 Resp: 43328

Ion	Ratio	Lower	Upper
164	100		
129	95.6	66.8	124.2
131	93.9	66.4	123.4
166	127.6	91.7	170.3

