

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041522\
 Data File : VW025593.D
 Acq On : 16 Apr 2022 02:15
 Operator : SY/MD
 Sample : N2438-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T0

Quant Time: Apr 16 04:50:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 16 04:36:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	120217	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	122102	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54184	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	41177	3.684	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.600%
7) Chloroethane-d5	1.571	69	43374	3.648	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.000%
11) 1,1-Dichloroethene-d2	2.111	63	64199	2.867	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.400%#
20) 2-Butanone-d5	3.896	46	72219	53.120	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.240%
24) Chloroform-d	4.352	84	75155	4.450	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.034	65	37309	5.127	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.053	84	141041	3.992	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.800%
36) 1,2-Dichloropropane-d6	6.069	67	45606	4.629	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.600%
41) Toluene-d8	7.317	98	111515	3.401	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.000%#
43) trans-1,3-Dichloroprop...	7.629	79	11756	3.550	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.000%
46) 2-Hexanone-d5	8.088	63	54371	46.779	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.560%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29273	4.703	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	39510	4.349	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.000%
Target Compounds						Qvalue
14) Carbon disulfide	2.298	76	3620	0.145	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025593.D
Acq On : 16 Apr 2022 02:15
Operator : SY/MD
Sample : N2438-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T0

Quant Time: Apr 16 04:50:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 16 04:36:16 2022
Response via : Initial Calibration

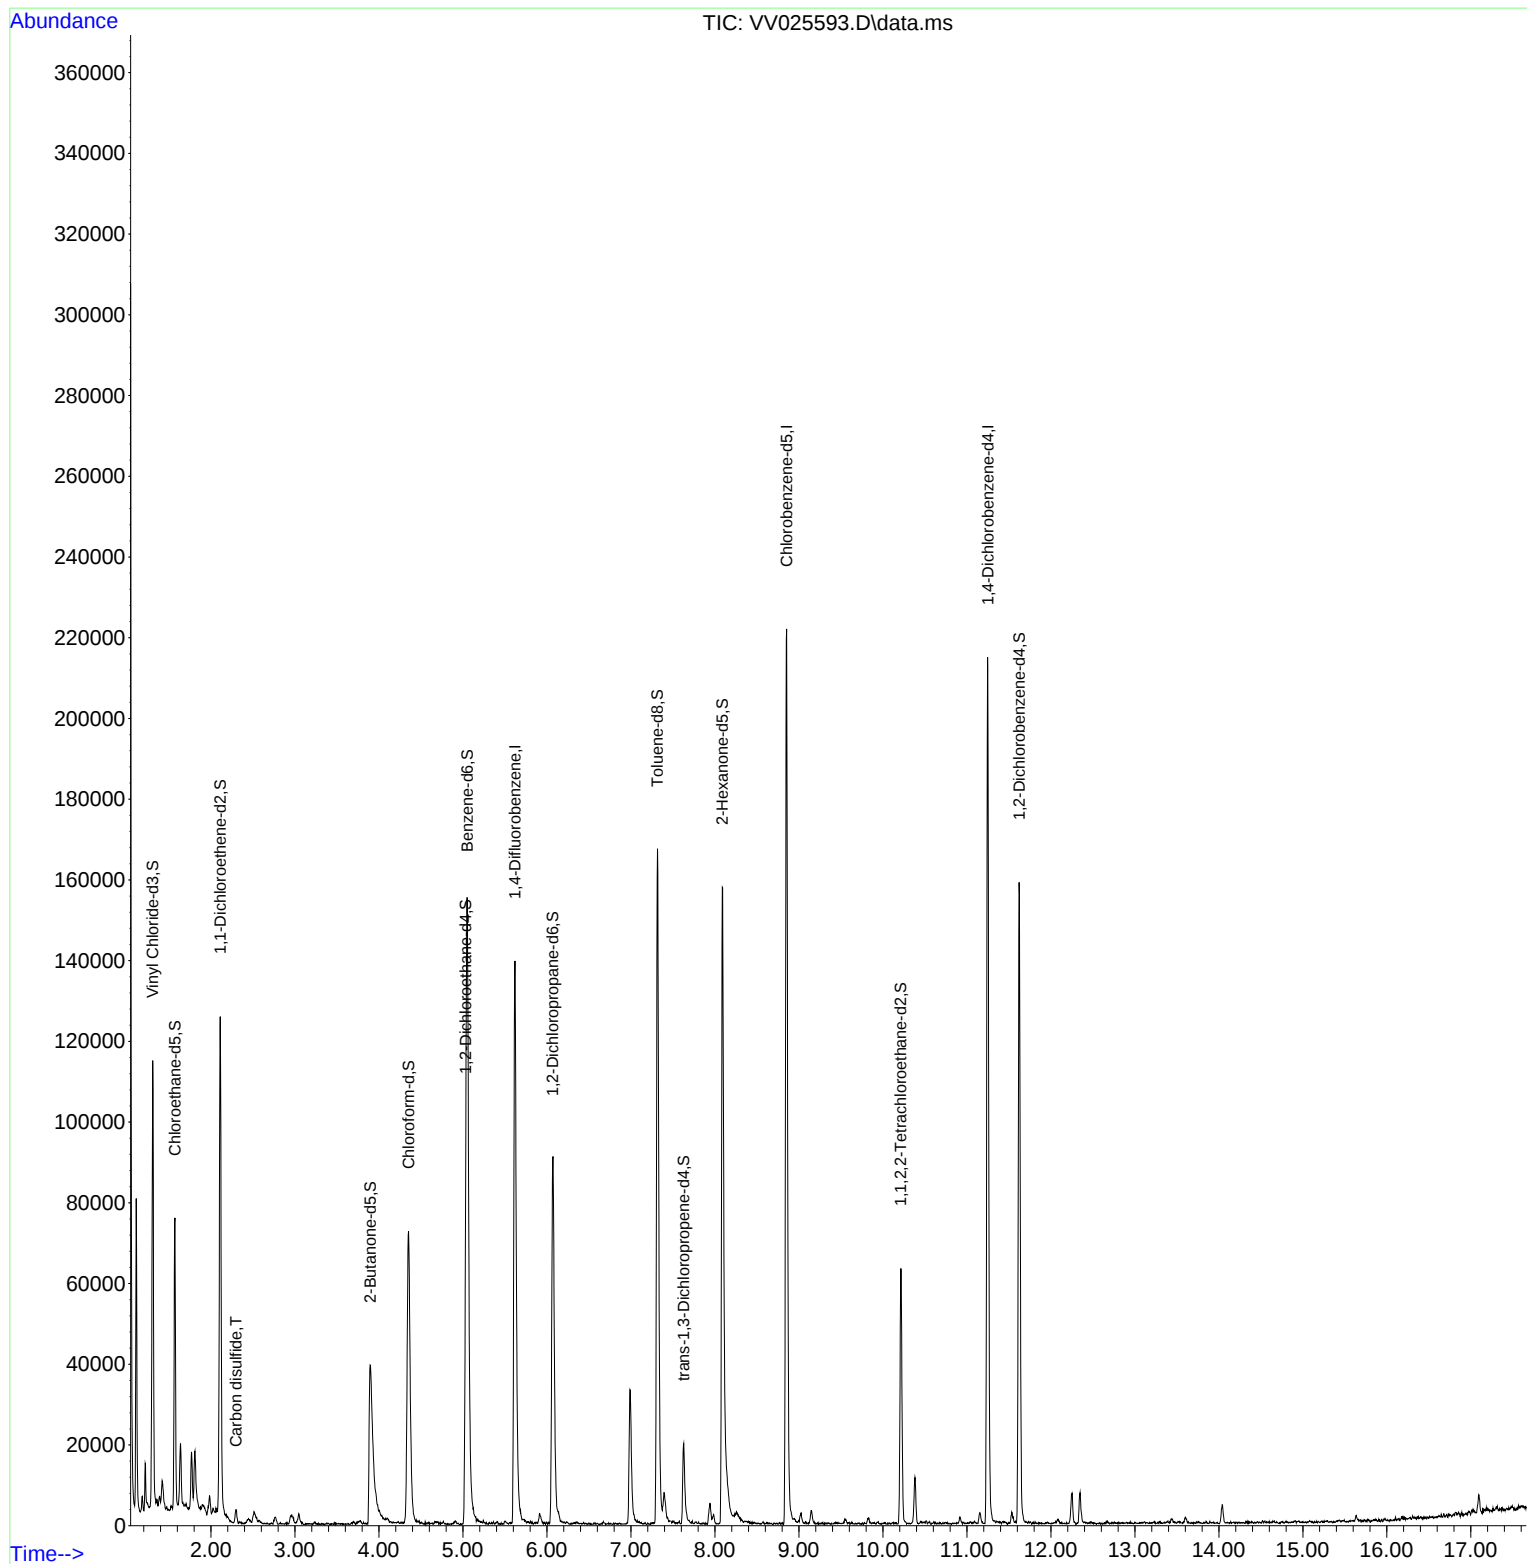

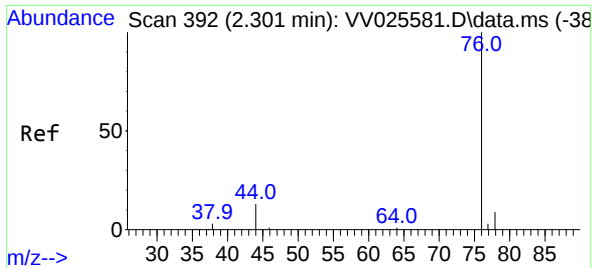

#14
Carbon disulfide
Concen: 0.145 ug/L
RT: 2.298 min Scan# 391
Delta R.T. -0.003 min
Lab File: VV025593.D
Acq: 16 Apr 2022 02:15

Instrument :
MSVOA_V
ClientSampleId :
EW6T0

Tgt Ion: 76 Resp: 3620
Ion Ratio Lower Upper
76 100
78 7.9 7.3 10.9

