

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
 Data File : VV025561.D
 Acq On : 15 Apr 2022 12:36
 Operator : SY/MD
 Sample : N2373-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	96	rBV	107071	107156	18.42%	2.155%
2	1.571	158	165	177	rVB	103283	114200	19.64%	2.296%
3	2.111	323	333	349	rVB	196091	286109	49.19%	5.753%
4	2.510	447	457	472	rBV	23404	40485	6.96%	0.814%
5	3.044	609	623	639	rBV8	5673	13003	2.24%	0.261%
6	3.902	880	890	928	rBV	42359	168776	29.02%	3.394%
7	4.349	1012	1029	1052	rBV	104777	265127	45.59%	5.331%
8	5.047	1230	1246	1270	rBV2	234579	581595	100.00%	11.695%
9	5.616	1408	1423	1458	rBV	210298	435127	74.82%	8.750%
10	5.908	1503	1514	1529	rBV6	7995	17150	2.95%	0.345%
11	6.066	1550	1563	1583	rBV2	134062	280445	48.22%	5.639%
12	6.985	1839	1849	1874	rBV2	55107	107911	18.55%	2.170%
13	7.313	1940	1951	1970	rBV	271990	477846	82.16%	9.609%
14	7.622	2039	2047	2064	rBV2	31104	56741	9.76%	1.141%
15	8.088	2182	2192	2223	rBV	195665	424034	72.91%	8.527%
16	8.850	2418	2429	2449	rBV	331026	548033	94.23%	11.020%
17	10.214	2842	2853	2870	rBV2	77697	125473	21.57%	2.523%
18	10.378	2895	2904	2914	rVB3	4130	6176	1.06%	0.124%
19	11.246	3163	3174	3194	rBV	333817	516384	88.79%	10.384%
20	11.622	3280	3291	3313	rBV	246129	392397	67.47%	7.890%
21	12.249	3474	3486	3496	rVB2	5735	8885	1.53%	0.179%




Sum of corrected areas: 4973053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025561.D
Acq On : 15 Apr 2022 12:36
Operator : SY/MD
Sample : N2373-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

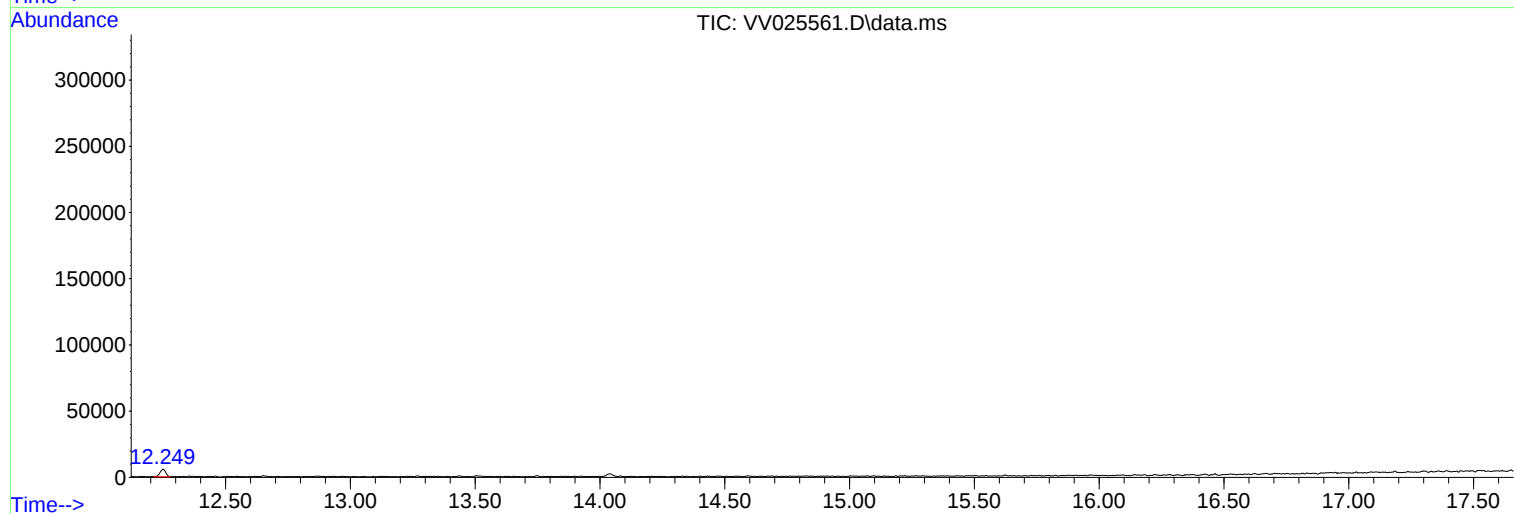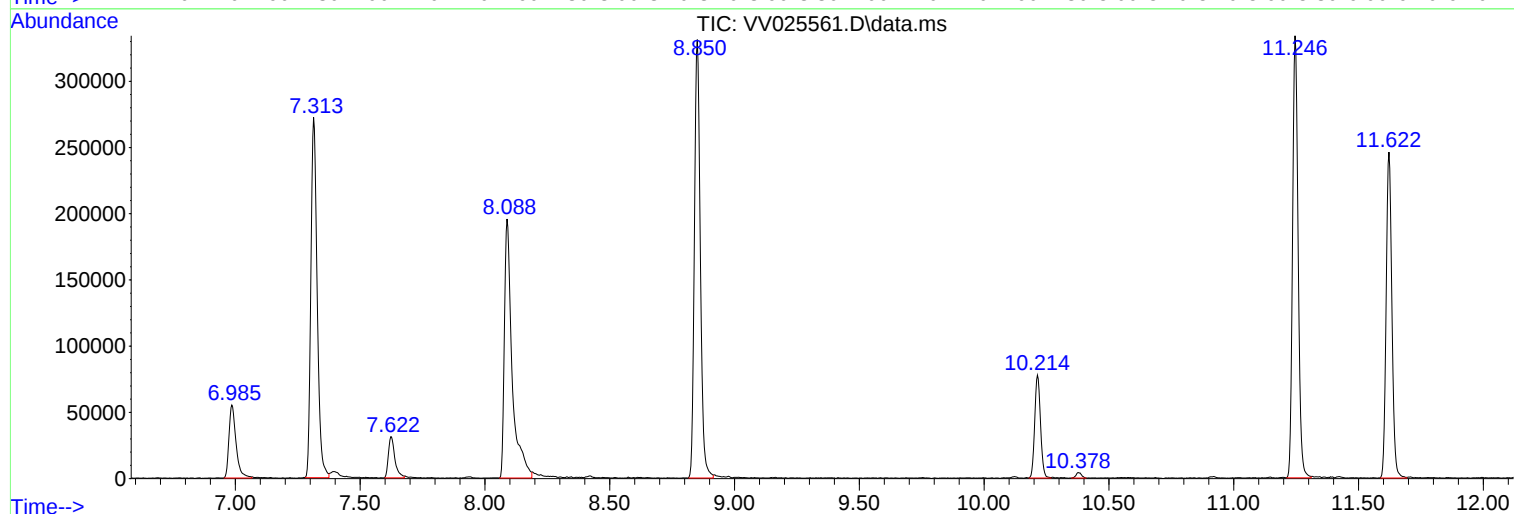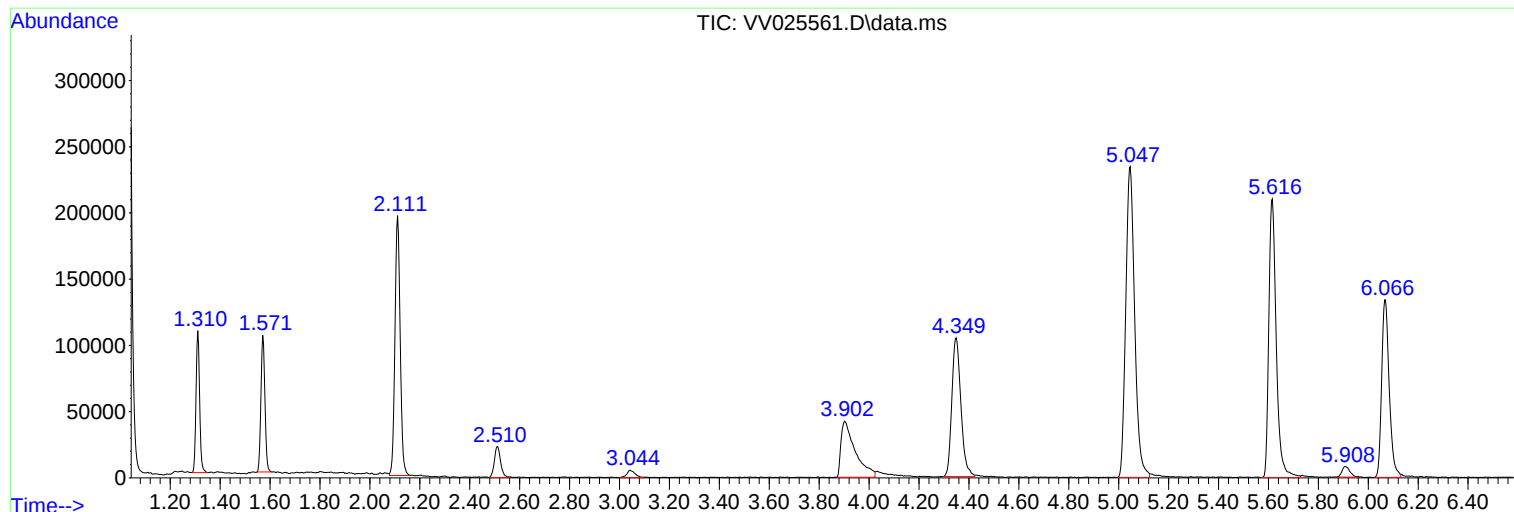

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025561.D
Acq On : 15 Apr 2022 12:36
Operator : SY/MD
Sample : N2373-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025561.D
Acq On : 15 Apr 2022 12:36
Operator : SY/MD
Sample : N2373-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
