

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
 Data File : VV025595.D
 Acq On : 16 Apr 2022 03:02
 Operator : SY/MD
 Sample : N2438-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025595.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	17	22	34	rVB	18274	19267	4.72%	0.558%
2	1.220	50	56	65	rBV2	10637	12367	3.03%	0.358%
3	1.310	75	84	94	rBV	77488	85183	20.86%	2.468%
4	1.571	156	165	176	rBV	73636	86386	21.15%	2.503%
5	1.642	180	187	192	rVB5	4707	6228	1.53%	0.180%
6	1.815	234	241	254	rVB9	3528	6421	1.57%	0.186%
7	2.111	323	333	353	rVB	128980	194422	47.61%	5.632%
8	2.510	450	457	469	rVB7	2203	4350	1.07%	0.126%
9	3.896	879	888	922	rBV	40949	133435	32.67%	3.866%
10	4.352	1012	1030	1057	rBV	76911	192811	47.21%	5.586%
11	5.050	1232	1247	1283	rBV2	159846	408391	100.00%	11.831%
12	5.619	1407	1424	1444	rBV	131563	270942	66.34%	7.849%
13	5.918	1509	1517	1528	rBV5	2934	4976	1.22%	0.144%
14	6.072	1551	1565	1590	rBV	95929	200161	49.01%	5.799%
15	6.989	1838	1850	1877	rBV2	34500	69491	17.02%	2.013%
16	7.317	1940	1952	1972	rBV	174793	311359	76.24%	9.020%
17	7.400	1972	1978	1986	rVB3	4277	6680	1.64%	0.194%
18	7.629	2041	2049	2064	rBV	20499	36656	8.98%	1.062%
19	7.944	2138	2147	2154	rBV4	3194	4785	1.17%	0.139%
20	8.092	2179	2193	2226	rBV	159865	317832	77.83%	9.208%
21	8.854	2419	2430	2455	rBV	220568	362898	88.86%	10.513%
22	10.217	2842	2854	2870	rBV	67292	106018	25.96%	3.071%
23	10.378	2895	2904	2914	rBV3	8859	14011	3.43%	0.406%
24	11.249	3163	3175	3196	rBV	207022	319247	78.17%	9.249%
25	11.622	3279	3291	3310	rBV	163290	263730	64.58%	7.640%
26	12.249	3477	3486	3498	rVB2	5537	9299	2.28%	0.269%
27	17.091	4987	4992	5000	rBV3	3231	4461	1.09%	0.129%




Sum of corrected areas: 3451807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025595.D
Acq On : 16 Apr 2022 03:02
Operator : SY/MD
Sample : N2438-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

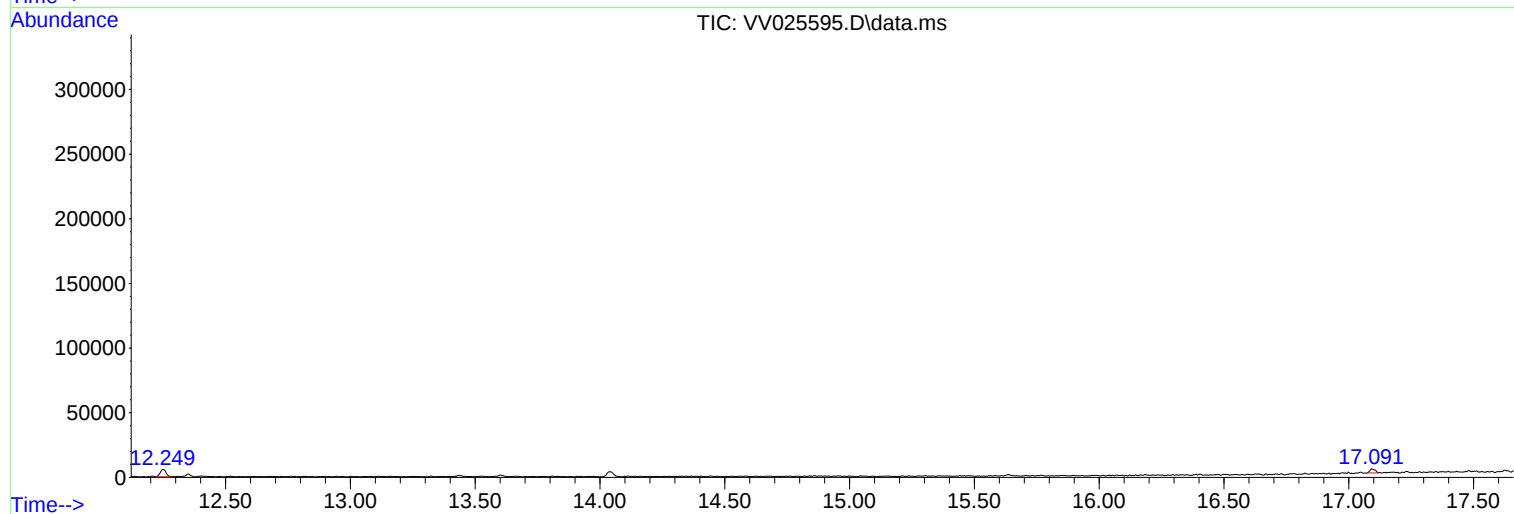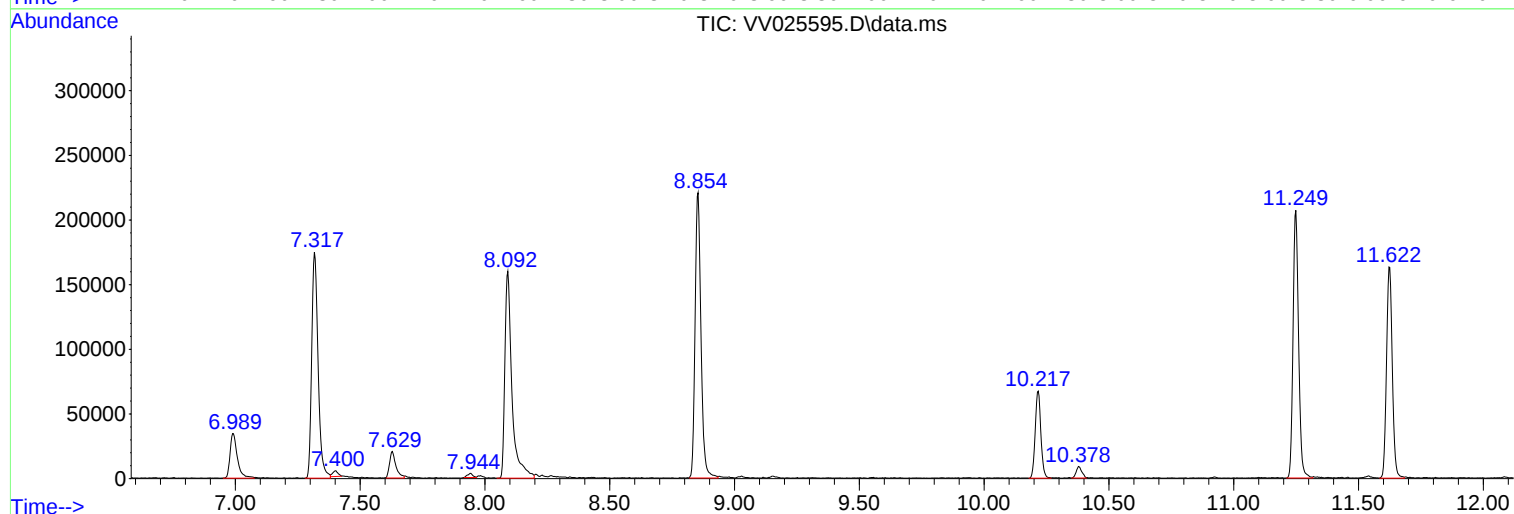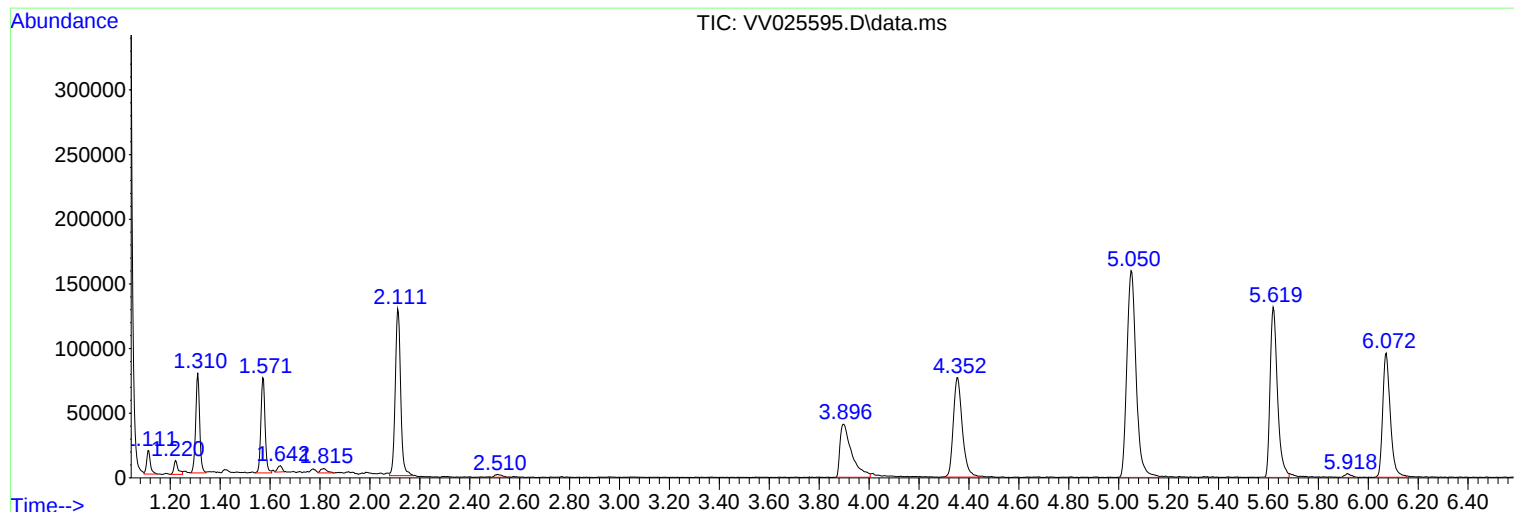

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025595.D
Acq On : 16 Apr 2022 03:02
Operator : SY/MD
Sample : N2438-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
Data File : VV025595.D
Acq On : 16 Apr 2022 03:02
Operator : SY/MD
Sample : N2438-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
