


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041522\
 Data File : VV025558.D
 Acq On : 15 Apr 2022 09:50
 Operator : SY/MD
 Sample : BFB303
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB303

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Apr 19 05:06:28 2022

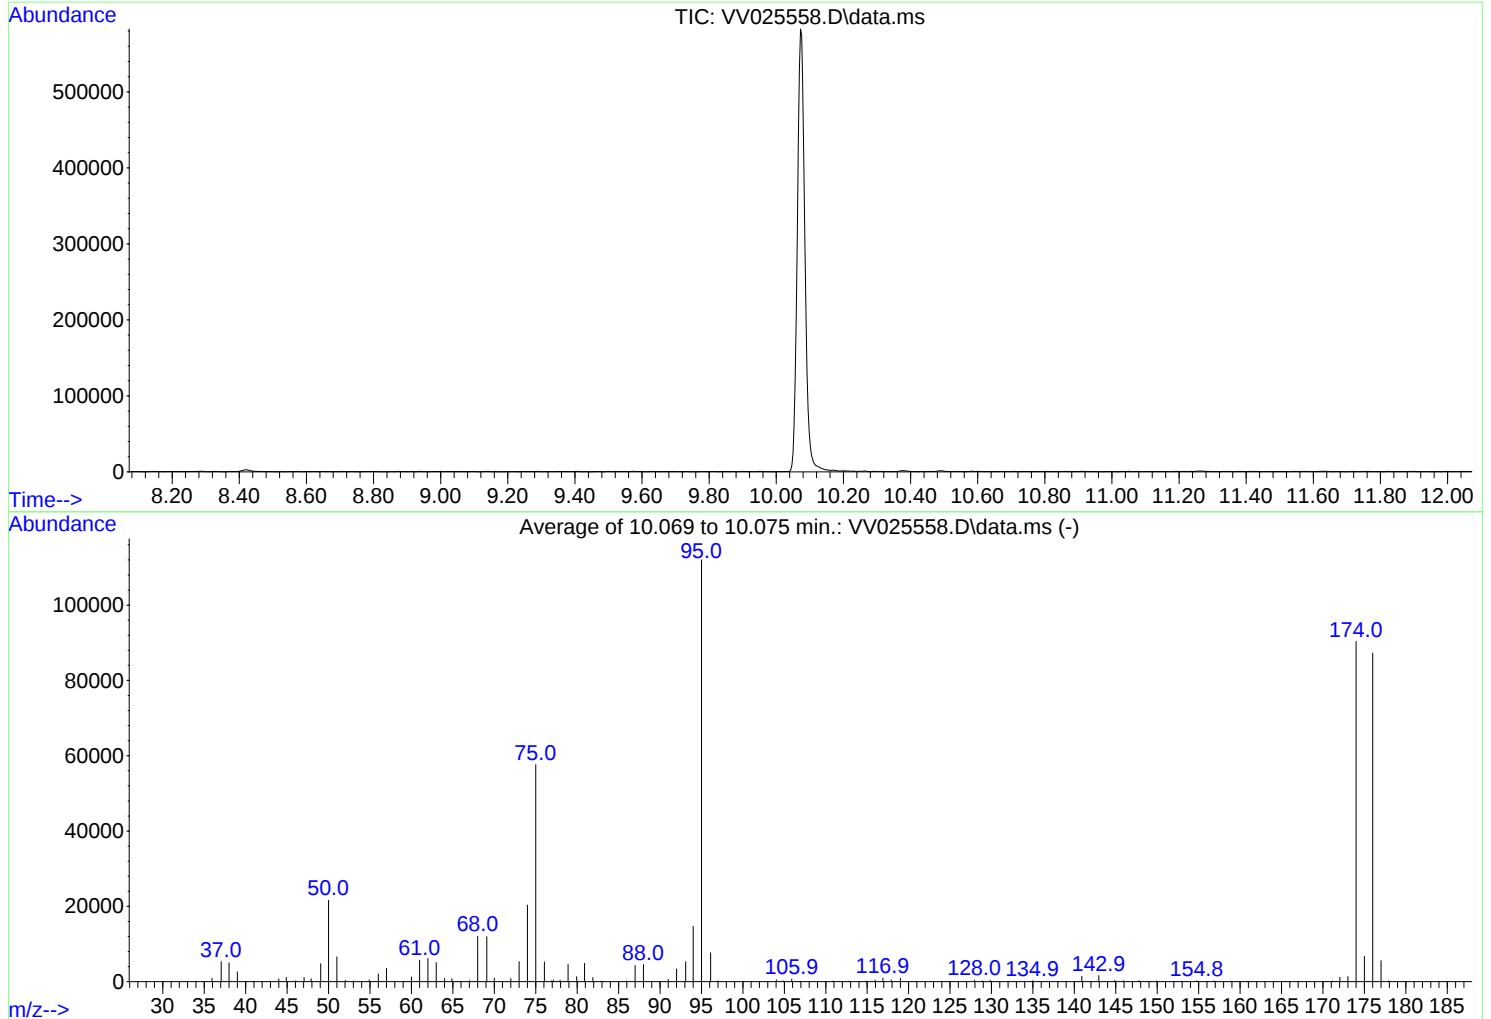

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	21605	PASS
75	95	30	80	51.5	57640	PASS
95	95	100	100	100.0	112029	PASS
96	95	5	9	6.8	7659	PASS
173	174	0.00	2	1.5	1353	PASS
174	95	50	120	80.7	90368	PASS
175	174	5	9	7.4	6727	PASS
176	174	95	105	96.5	87235	PASS
177	176	5	10	6.4	5558	PASS

m/z	Abundance
40.00	189.0
44.00	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
35.90	851.0
37.10	5039.0
38.00	4924.0
39.00	2491.0
40.10	214.0
40.90	132.0
43.00	113.0
44.00	973.0
44.90	1078.0
46.10	230.0
47.10	955.0
47.90	722.0
49.10	4586.0
50.00	20640.0
51.00	6506.0
52.00	338.0
53.10	164.0
54.90	456.0
56.00	1926.0
57.00	3210.0
57.90	116.0
60.00	1156.0
61.00	5380.0
62.00	5720.0
63.00	4924.0
64.00	761.0
64.90	796.0
65.90	134.0
67.10	302.0
68.00	11559.0
69.10	11284.0
70.00	864.0
72.00	752.0
73.00	5127.0
74.00	19632.0
75.00	55024.0
76.00	5088.0
77.10	574.0
78.00	473.0
78.90	4340.0
79.90	1292.0
80.90	4663.0
81.90	1066.0
85.90	146.0
87.00	4099.0
88.00	4405.0
91.00	575.0
92.00	2973.0
93.10	5172.0
94.00	14042.0
95.00	107184.0
96.10	7467.0
97.10	208.0
104.10	454.0
104.80	201.0
105.90	665.0
110.80	160.0
112.80	145.0
114.90	196.0
116.00	437.0
116.90	922.0
117.90	466.0
119.00	758.0
127.90	371.0
128.90	255.0
129.80	341.0
130.80	146.0
135.00	211.0
136.80	129.0
140.90	1394.0
142.00	191.0
143.00	1497.0
144.10	121.0
144.90	330.0
145.90	208.0
147.80	270.0
148.80	117.0
149.90	160.0
153.00	118.0
154.80	185.0
156.90	156.0
158.90	165.0
160.80	119.0
170.40	105.0
171.10	234.0
172.00	1105.0
173.00	1241.0
174.00	83200.0
175.00	6207.0
176.00	80592.0
177.00	5227.0
178.00	258.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
35.90	938.0
37.00	5484.0
38.00	5147.0
39.00	2718.0
40.00	194.0
40.90	179.0
42.90	146.0
44.00	1058.0
44.90	1140.0
46.00	255.0
47.00	1091.0
47.90	776.0
49.00	4894.0
50.00	22344.0
51.00	6818.0
52.10	328.0
53.00	153.0
54.90	446.0
56.00	2087.0
57.00	3642.0
57.90	159.0
60.00	1292.0
61.00	5916.0
62.00	6398.0
63.00	5227.0
64.00	822.0
64.90	817.0
65.90	108.0
67.10	339.0
68.00	12443.0
69.10	12312.0
70.00	945.0
72.00	843.0
73.00	5425.0
74.00	20952.0
75.00	59664.0
76.00	5407.0
77.20	663.0
77.90	442.0
78.90	4743.0
79.90	1331.0
80.90	5067.0
81.90	1125.0
82.80	130.0
83.20	127.0
85.90	241.0
87.00	4401.0
88.00	4674.0
91.00	608.0
92.00	3480.0
93.10	5520.0
94.00	15042.0
95.00	116096.0
96.10	7929.0
97.00	234.0
104.10	501.0
104.80	214.0
105.90	734.0
110.80	174.0
112.80	144.0
114.80	166.0
115.90	436.0
116.90	980.0
117.90	498.0
119.00	920.0
127.90	457.0
128.90	241.0
129.90	404.0
130.80	133.0
134.90	259.0
135.70	102.0
137.00	164.0
140.90	1499.0
143.00	1659.0
144.10	115.0
144.90	332.0
145.90	271.0
147.80	343.0
148.80	109.0
149.90	170.0
153.00	121.0
154.80	249.0
156.80	241.0
158.90	162.0
160.90	104.0
161.20	110.0
170.40	105.0
171.20	248.0
172.10	1186.0
173.00	1419.0
174.00	93656.0
175.00	6978.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

176.00	90328.0
177.00	5716.0
177.90	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	954.0
37.00	5476.0
38.00	4947.0
39.00	2519.0
40.10	203.0
40.90	141.0
42.90	140.0
44.00	1029.0
44.90	1089.0
46.00	264.0
47.00	1252.0
47.90	781.0
49.00	4767.0
50.00	21832.0
51.00	6483.0
52.10	341.0
53.00	174.0
54.90	352.0
56.00	2063.0
57.00	3655.0
58.00	173.0
60.00	1283.0
61.00	5834.0
62.00	6402.0
63.00	5049.0
64.00	803.0
64.90	862.0
67.00	328.0
68.00	12170.0
69.10	12184.0
70.00	954.0
71.10	103.0
72.00	821.0
73.00	5365.0
74.00	20312.0
75.00	58232.0
76.10	5152.0
76.90	618.0
77.90	360.0
78.90	4725.0
80.00	1286.0
80.90	4870.0
81.90	1089.0
82.80	127.0
83.20	152.0
86.00	305.0
87.00	4438.0
88.00	4519.0
91.00	605.0
92.00	3612.0
93.10	5073.0
94.00	14858.0
95.00	112808.0
96.10	7581.0
96.90	221.0
104.00	477.0
104.90	187.0
105.90	667.0
106.90	107.0
109.90	108.0
110.90	170.0
112.70	132.0
114.80	160.0
115.90	419.0
116.90	913.0
117.90	485.0
119.00	868.0
128.00	498.0
128.90	196.0
129.90	427.0
131.00	153.0
134.90	288.0
137.00	193.0
140.90	1484.0
142.90	1717.0
144.00	116.0
144.90	329.0
145.90	298.0
147.80	339.0
149.90	157.0
152.90	111.0
154.80	304.0
156.80	290.0
158.90	134.0
161.10	126.0
172.10	1124.0
173.00	1398.0
174.00	94248.0
175.00	6996.0
176.00	90784.0
177.00	5730.0
177.90	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303