

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041524\
 Data File : VW035205.D
 Acq On : 15 Apr 2024 18:30
 Operator : SY/MD
 Sample : P2057-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ3

Quant Time: Apr 16 01:48:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 16 00:33:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	165609	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	167788	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	74921	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	83042	5.355	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.200%
7) Chloroethane-d5	1.532	69	65211	5.413	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.200%
11) 1,1-Dichloroethene-d2	2.060	65	34663	5.269	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	105.400%
20) 2-Butanone-d5	3.812	46	173973	66.329	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.660%#
24) Chloroform-d	4.253	84	127100	5.242	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%
26) 1,2-Dichloroethane-d4	4.947	65	68093	5.900	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.000%
32) Benzene-d6	4.960	84	254559	5.340	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.800%
36) 1,2-Dichloropropane-d6	5.989	67	82063	5.536	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.800%
41) Toluene-d8	7.246	98	204550	4.778	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.600%
43) trans-1,3-Dichloroprop...	7.561	79	26952	5.094	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.800%
46) 2-Hexanone-d5	8.027	63	126356	57.343	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.680%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	65165	5.707	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	73407	5.512	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.200%
Target Compounds						Qvalue
47) Tetrachloroethene	7.908	164	5462	0.496	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035205.D
Acq On : 15 Apr 2024 18:30
Operator : SY/MD
Sample : P2057-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ3


Quant Time: Apr 16 01:48:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 16 00:33:27 2024
Response via : Initial Calibration

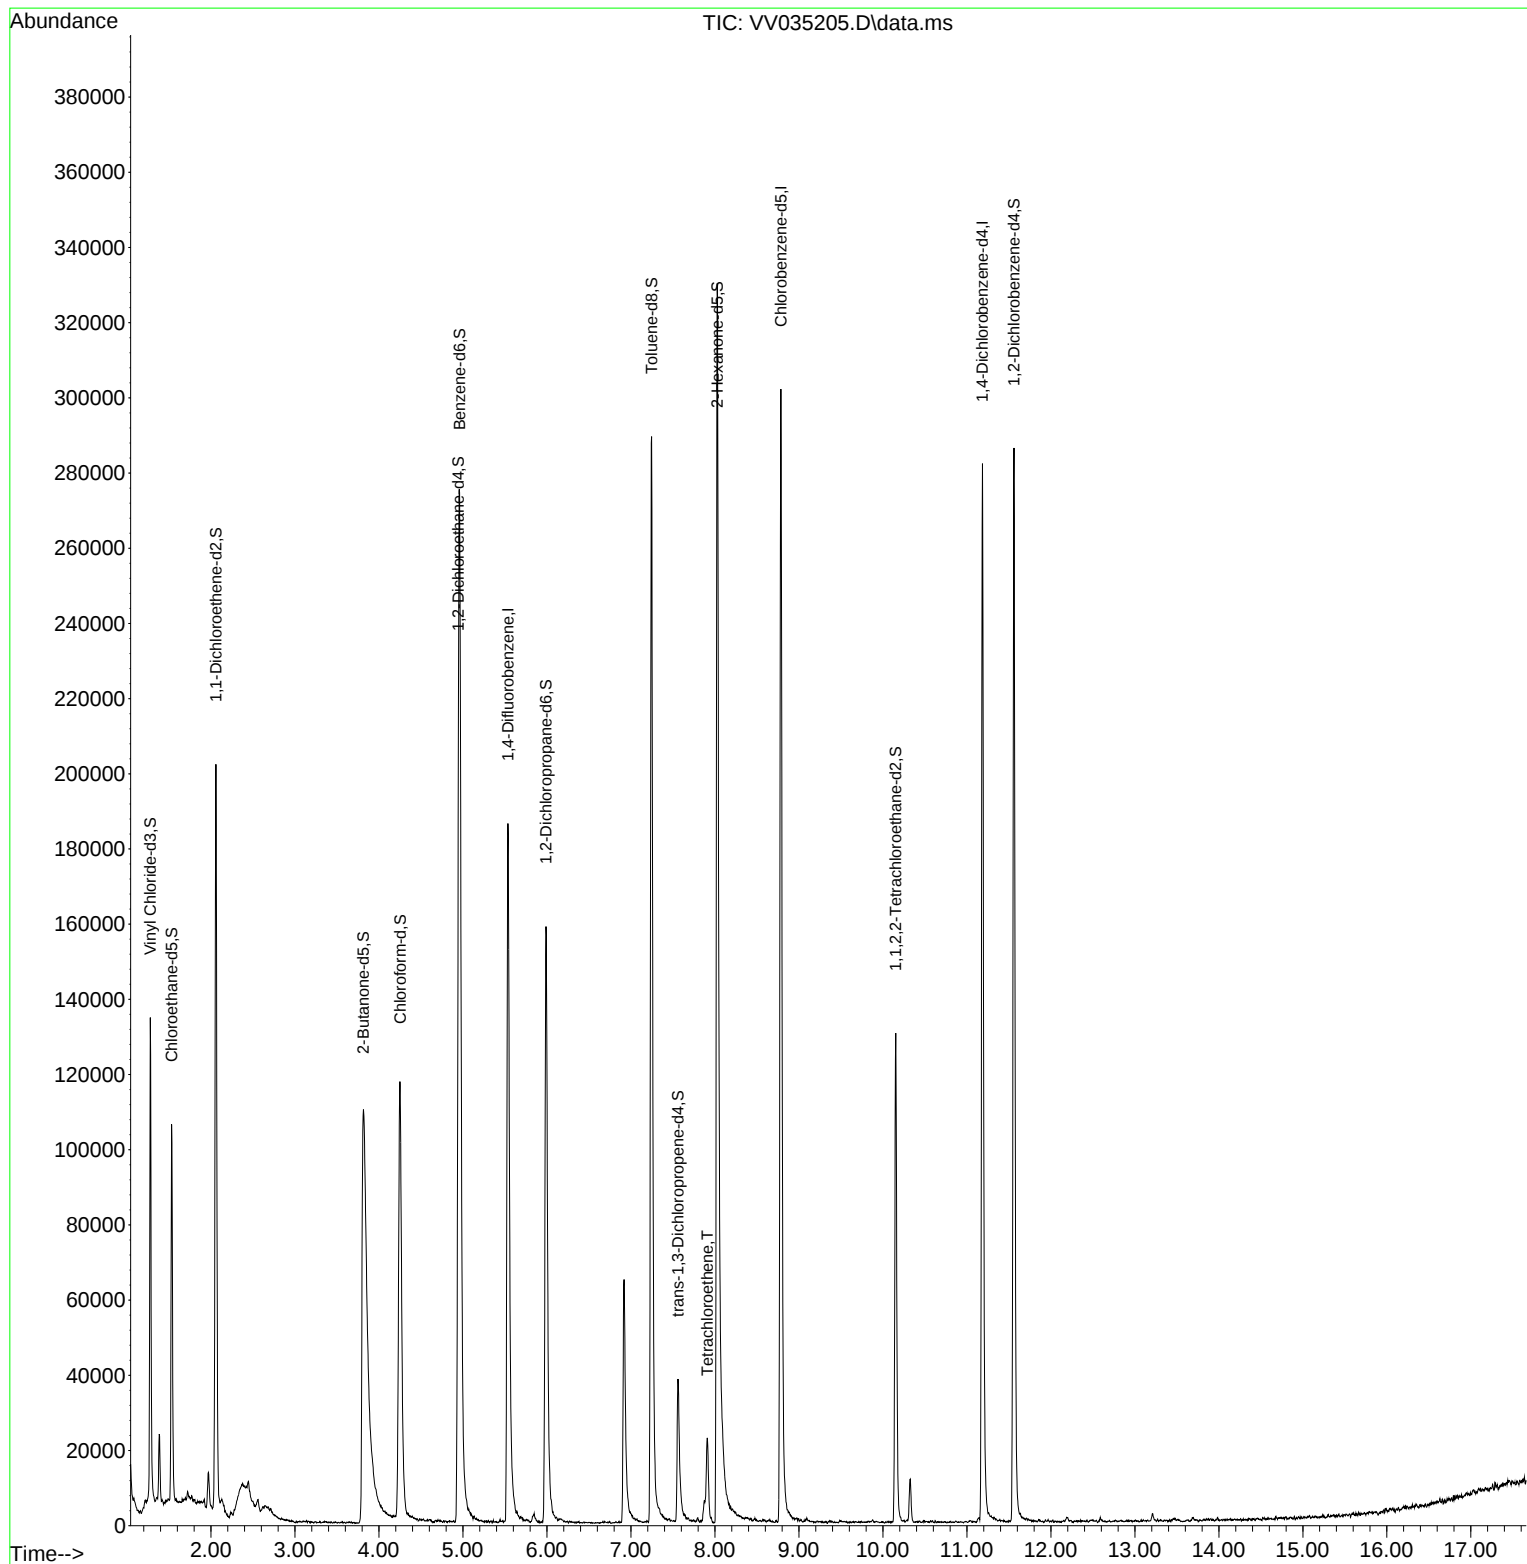

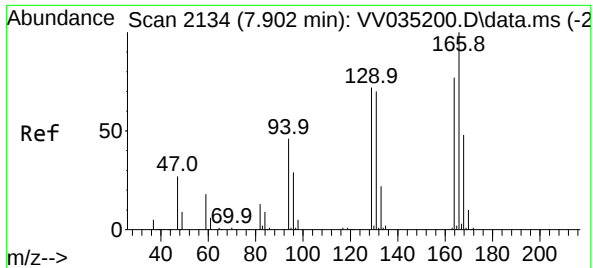

#47
 Tetrachloroethene
 Concen: 0.496 ug/L
 RT: 7.908 min Scan# 2136
 Delta R.T. 0.006 min
 Lab File: VV035205.D
 Acq: 15 Apr 2024 18:30

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ3

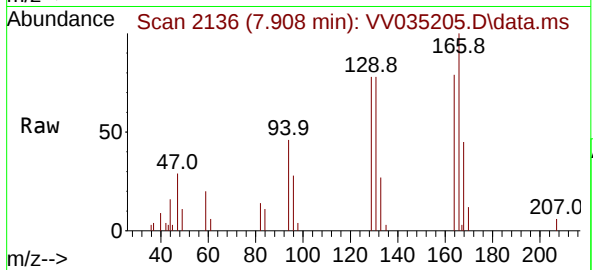

Tgt Ion:	164	Resp:	5462
Ion	Ratio	Lower	Upper
164	100		
129	98.8	65.3	121.3
131	98.5	60.9	113.1
166	126.2	87.4	162.4

