

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041524\
 Data File : VW035209.D
 Acq On : 15 Apr 2024 20:06
 Operator : SY/MD
 Sample : P2057-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 16 01:49:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 16 00:33:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	184619	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	190386	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	81004	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	87614	5.068	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.400%
7) Chloroethane-d5	1.532	69	71230	5.303	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.000%
11) 1,1-Dichloroethene-d2	2.057	65	37923	5.171	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.400%
20) 2-Butanone-d5	3.828	46	161647	55.284	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.560%
24) Chloroform-d	4.249	84	139841	5.174	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
26) 1,2-Dichloroethane-d4	4.944	65	72095	5.604	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.000%
32) Benzene-d6	4.960	84	275804	5.099	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
36) 1,2-Dichloropropane-d6	5.989	67	90325	5.370	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.400%
41) Toluene-d8	7.243	98	227186	4.677	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
43) trans-1,3-Dichloroprop...	7.561	79	26612	4.433	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.600%
46) 2-Hexanone-d5	8.031	63	116774	46.704	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.400%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	64611	4.987	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	79369	5.512	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.200%
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	5123	0.290	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035209.D
Acq On : 15 Apr 2024 20:06
Operator : SY/MD
Sample : P2057-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Apr 16 01:49:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 16 00:33:27 2024
Response via : Initial Calibration

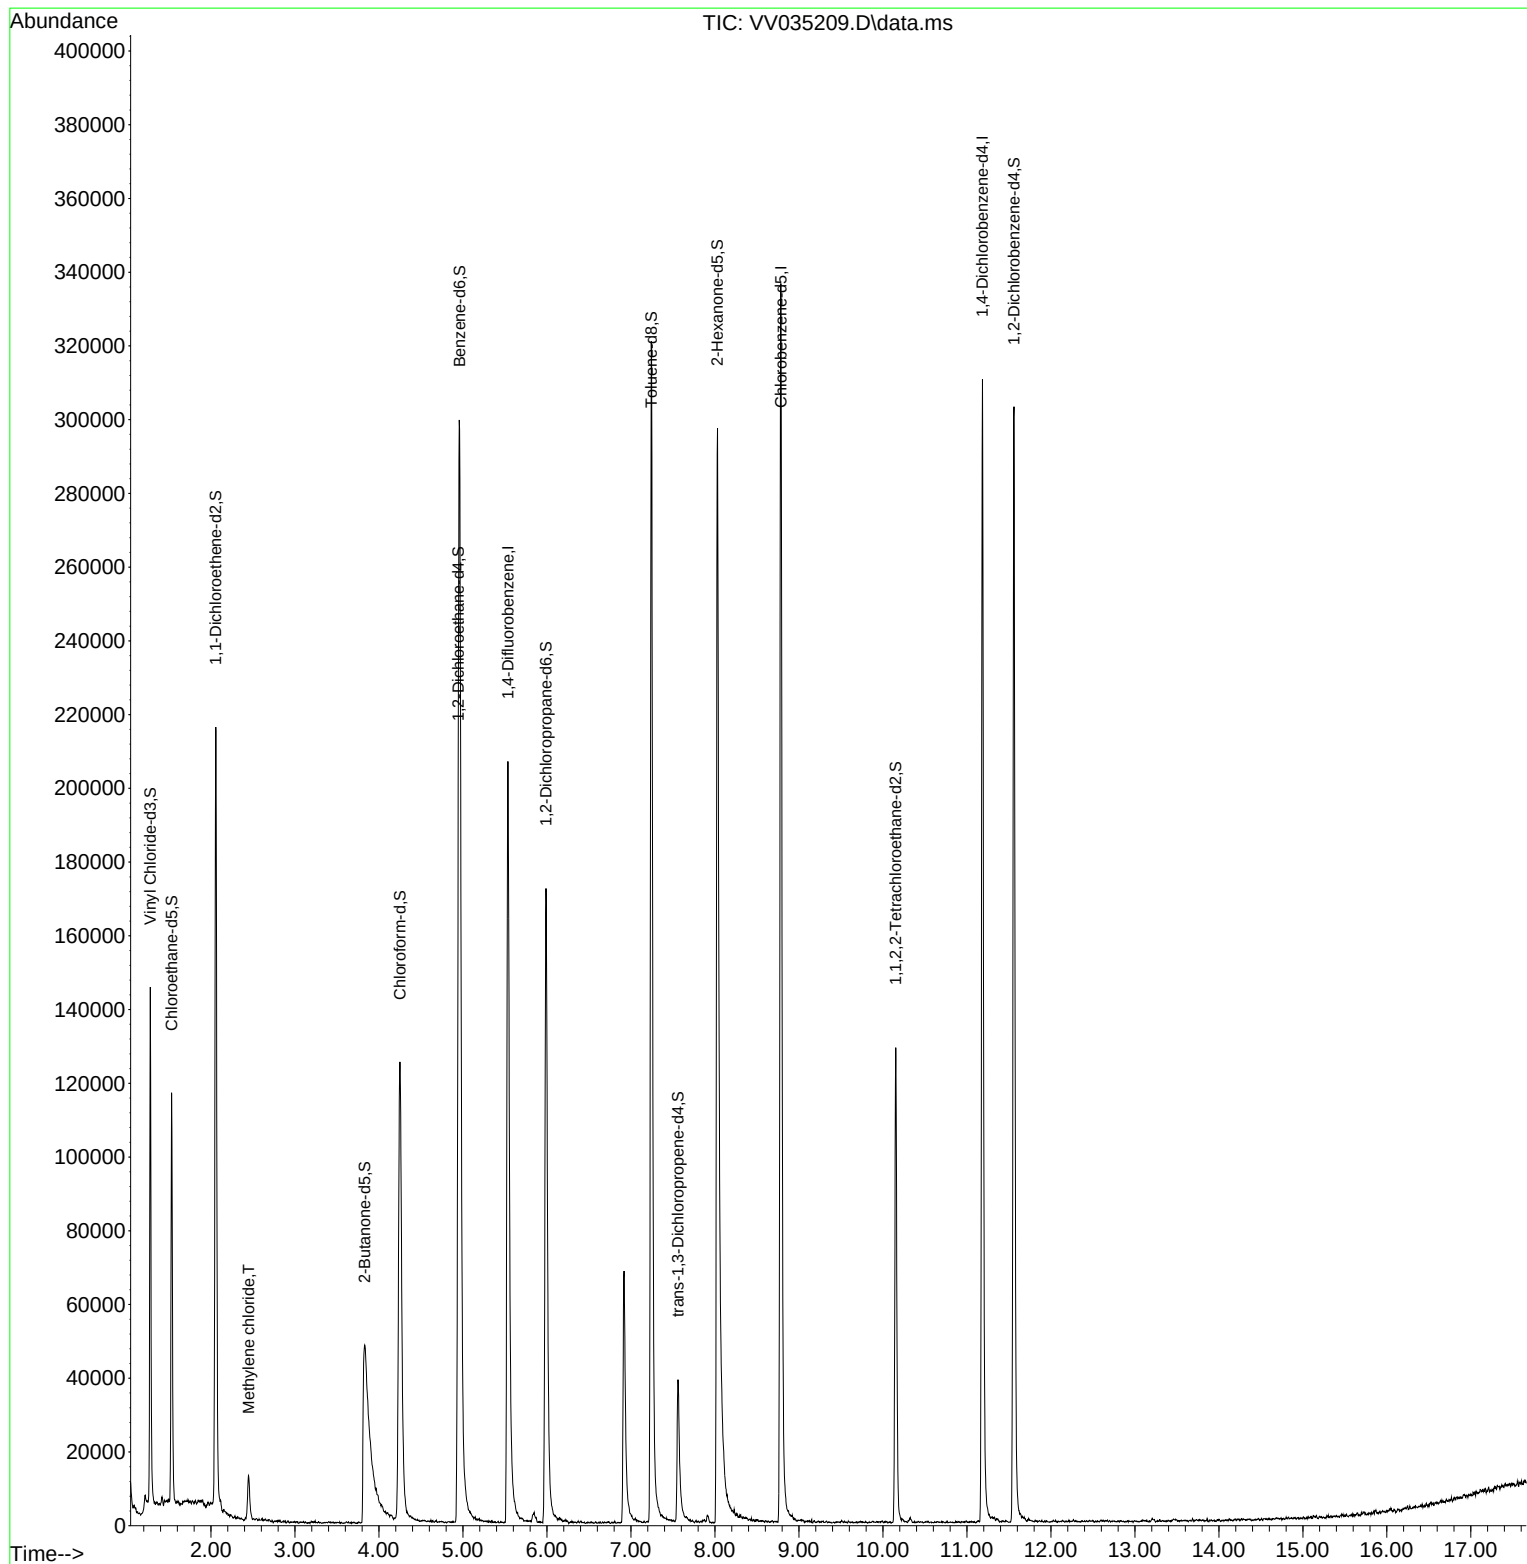

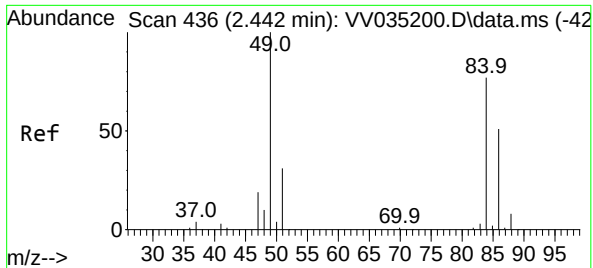

#16
Methylene chloride
Concen: 0.290 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.007 min
Lab File: VV035209.D
Acq: 15 Apr 2024 20:06

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84	Resp: 5123
Ion Ratio	Lower Upper
84 100	
86 61.6	45.6 84.6
49 122.5	89.5 166.1

