

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041524\
 Data File : VW035210.D
 Acq On : 15 Apr 2024 20:30
 Operator : SY/MD
 Sample : P2032-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0ME7

Quant Time: Apr 16 01:49:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 16 00:33:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	186014	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	187569	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	80671	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	89681	5.149	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.000%
7) Chloroethane-d5	1.532	69	70803	5.232	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.600%
11) 1,1-Dichloroethene-d2	2.060	65	36713	4.969	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	99.400%
20) 2-Butanone-d5	3.812	46	171138	58.091	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.180%
24) Chloroform-d	4.249	84	143281	5.261	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.200%
26) 1,2-Dichloroethane-d4	4.944	65	72356	5.582	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.600%
32) Benzene-d6	4.960	84	275708	5.174	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
36) 1,2-Dichloropropane-d6	5.989	67	90831	5.481	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.600%
41) Toluene-d8	7.246	98	222084	4.640	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
43) trans-1,3-Dichloroprop...	7.561	79	27016	4.568	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.027	63	120873	49.070	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.140%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	66876	5.239	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	79823	5.567	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.400%
Target Compounds						
					Qvalue	
29) 1,1,1-Trichloroethane	4.513	97	39599	1.678	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035210.D
Acq On : 15 Apr 2024 20:30
Operator : SY/MD
Sample : P2032-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOME7

Quant Time: Apr 16 01:49:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 16 00:33:27 2024
Response via : Initial Calibration

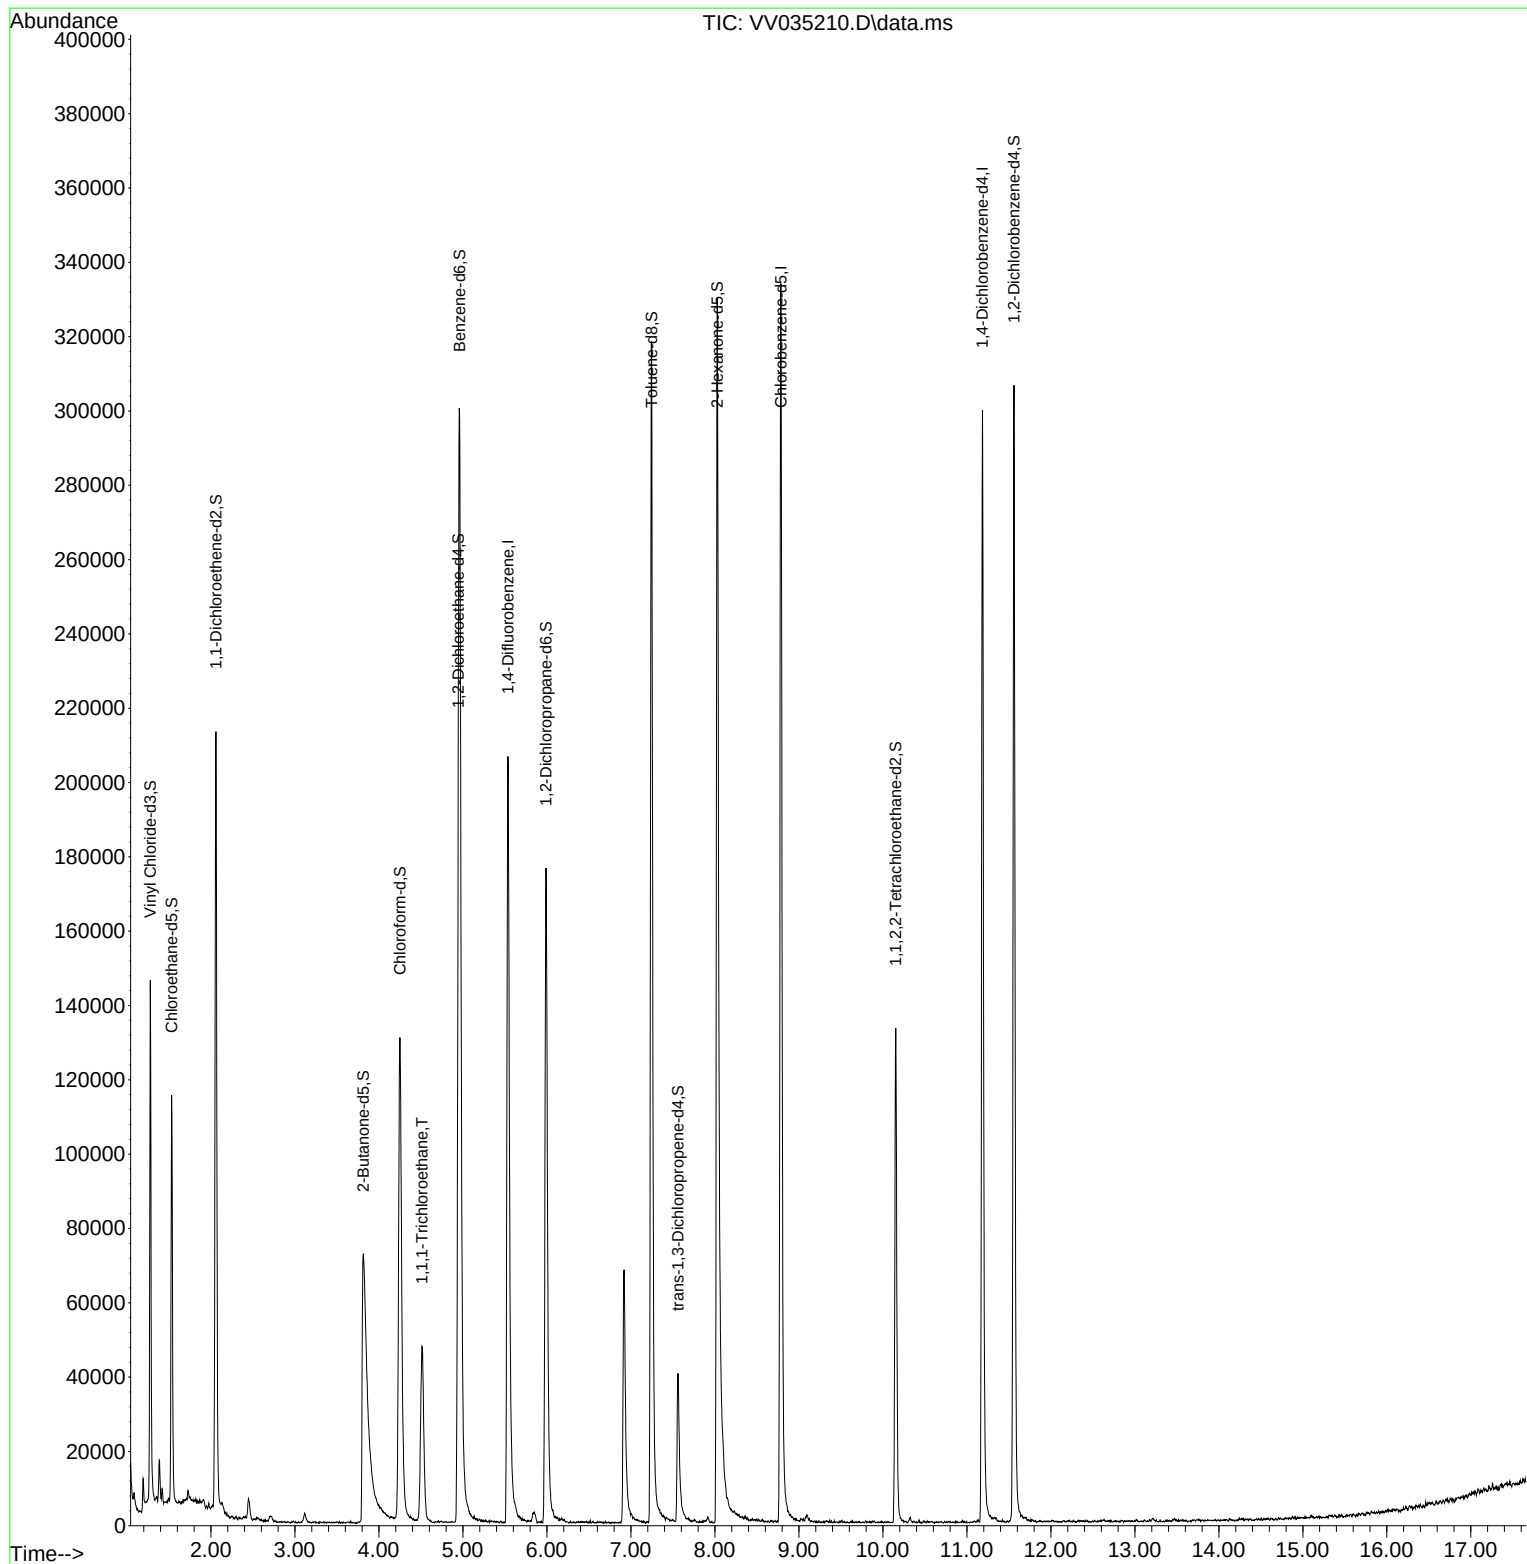

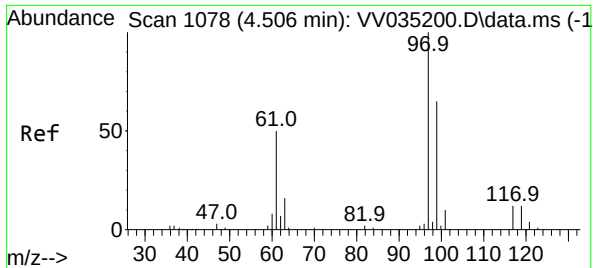

#29
 1,1,1-Trichloroethane
 Concen: 1.678 ug/L
 RT: 4.513 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV035210.D
 Acq: 15 Apr 2024 20:30

Instrument :
 MSVOA_V
 ClientSampleId :
 E0ME7

Tgt Ion: 97 Resp: 39599

Ion	Ratio	Lower	Upper
97	100		
99	64.0	51.4	77.2
61	48.0	38.3	57.5

