

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
 Data File : VV035204.D
 Acq On : 15 Apr 2024 18:06
 Operator : SY/MD
 Sample : P2057-14DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	87	rBV	146345	152471	19.17%	2.122%
2	1.532	145	153	164	rBV	113677	133586	16.80%	1.859%
3	2.056	306	316	349	rVB	230578	351353	44.18%	4.890%
4	2.445	426	437	459	rBV	57043	99328	12.49%	1.382%
5	3.831	855	868	926	rBV2	50295	311619	39.18%	4.337%
6	4.249	983	998	1023	rBV	129467	332978	41.87%	4.634%
7	4.957	1204	1218	1243	rBV2	311867	795299	100.00%	11.069%
8	5.535	1386	1398	1426	rBV	210175	457783	57.56%	6.371%
9	5.989	1527	1539	1570	rBV	176308	382250	48.06%	5.320%
10	6.918	1816	1828	1850	rBV2	73413	150142	18.88%	2.090%
11	7.243	1918	1929	1961	rBV	340670	624491	78.52%	8.692%
12	7.561	2019	2028	2053	rBV2	43034	89829	11.29%	1.250%
13	7.905	2115	2135	2155	rBV	432472	745952	93.80%	10.382%
14	8.030	2164	2174	2228	rBV	315553	721790	90.76%	10.046%
15	8.786	2393	2409	2438	rBV	335990	585464	73.62%	8.148%
16	10.152	2823	2834	2854	rBV	129948	214622	26.99%	2.987%
17	10.326	2877	2888	2899	rVB	9399	15188	1.91%	0.211%
18	11.185	3144	3155	3177	rBV	314162	505162	63.52%	7.031%
19	11.561	3257	3272	3296	rBV	318873	515734	64.85%	7.178%




Sum of corrected areas: 7185041

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035204.D
Acq On : 15 Apr 2024 18:06
Operator : SY/MD
Sample : P2057-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

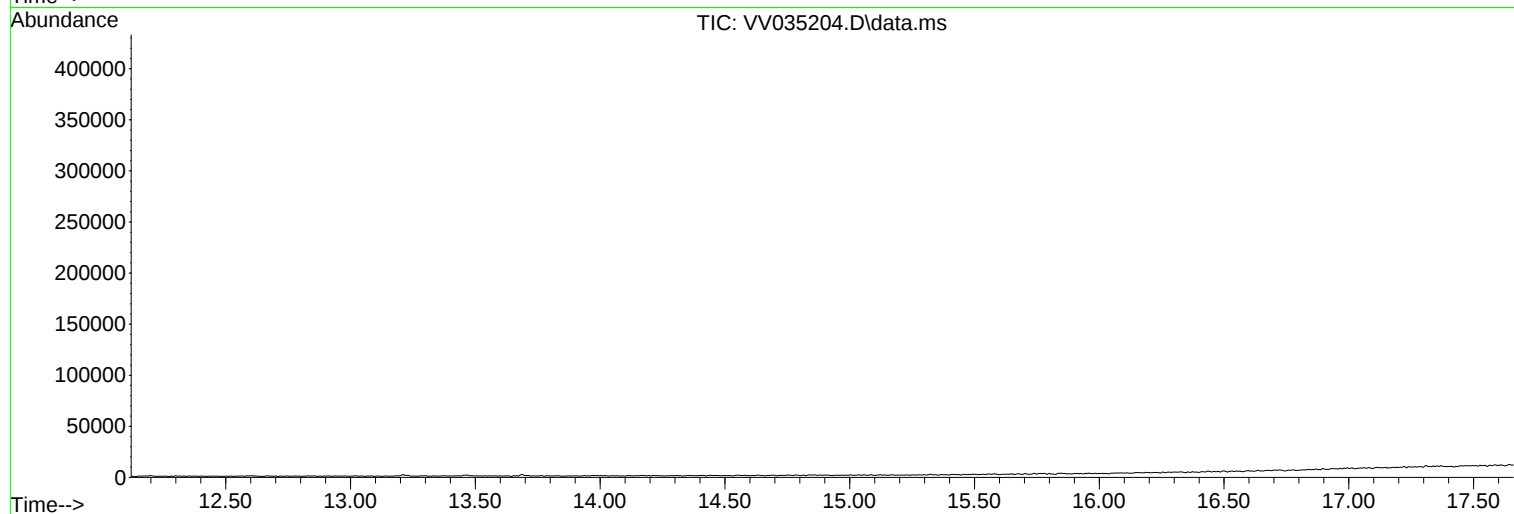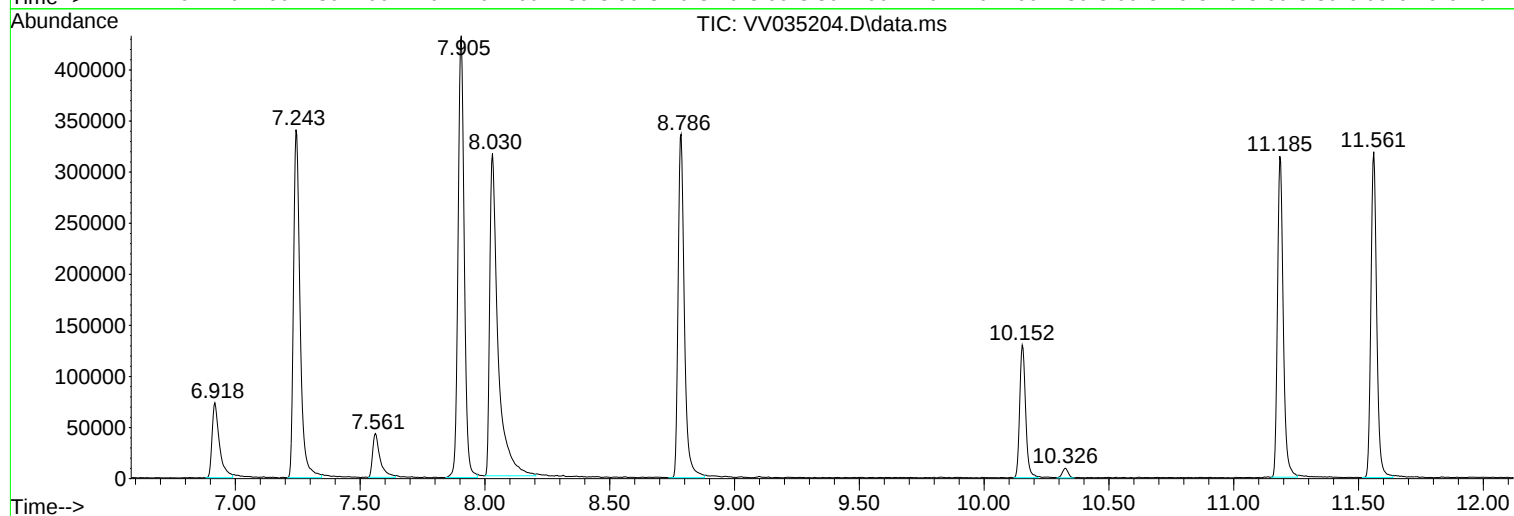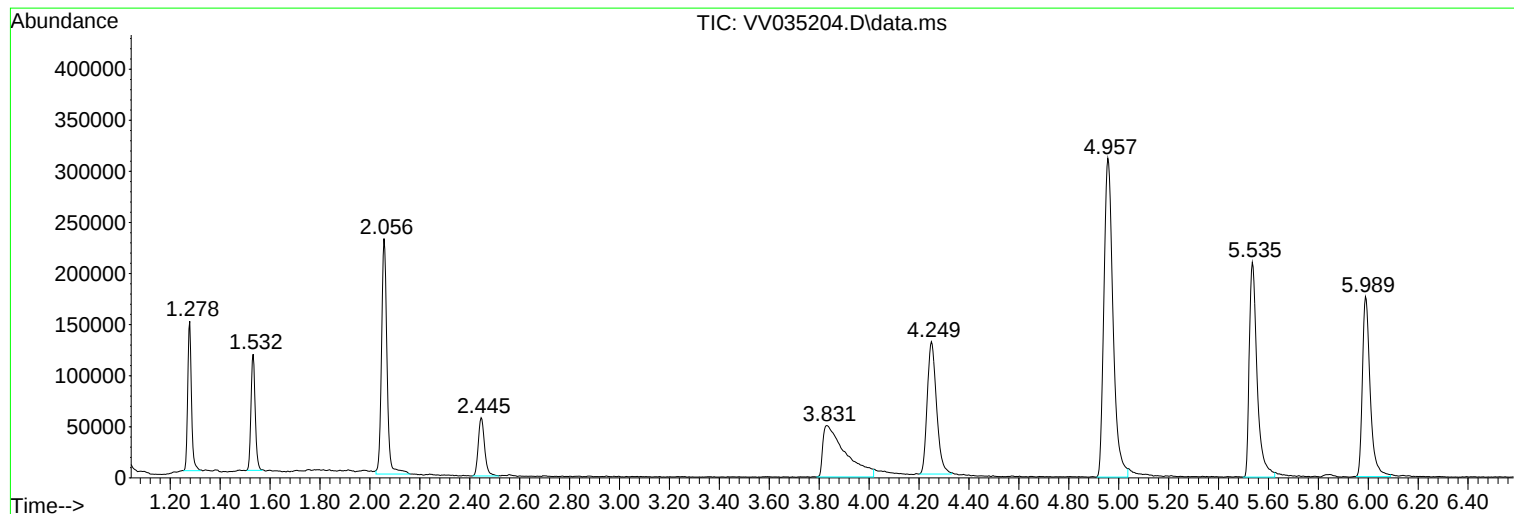

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035204.D
Acq On : 15 Apr 2024 18:06
Operator : SY/MD
Sample : P2057-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035204.D
Acq On : 15 Apr 2024 18:06
Operator : SY/MD
Sample : P2057-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc