

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
 Data File : VV035205.D
 Acq On : 15 Apr 2024 18:30
 Operator : SY/MD
 Sample : P2057-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	128734	140177	19.45%	2.318%
2	1.384	101	107	115	rVB	17921	20540	2.85%	0.340%
3	1.532	146	153	166	rVB	99945	117636	16.32%	1.945%
4	1.970	282	289	304	rVB	9682	15257	2.12%	0.252%
5	2.060	306	317	332	rBV	197640	287162	39.84%	4.749%
6	3.815	844	863	926	rBV3	110030	521172	72.30%	8.619%
7	4.249	983	998	1024	rBV	115702	298263	41.38%	4.932%
8	4.957	1201	1218	1252	rBV2	274970	718997	99.74%	11.890%
9	5.535	1388	1398	1429	rBV	185556	402299	55.81%	6.653%
10	5.989	1527	1539	1564	rBV	158233	339372	47.08%	5.612%
11	6.918	1817	1828	1848	rBV	64680	131067	18.18%	2.168%
12	7.246	1919	1930	1969	rBV	288788	542816	75.30%	8.977%
13	7.561	2018	2028	2052	rBV2	37871	80043	11.10%	1.324%
14	7.908	2129	2136	2150	rVB3	21567	39287	5.45%	0.650%
15	8.027	2164	2173	2215	rBV	329578	720852	100.00%	11.921%
16	8.786	2397	2409	2433	rBV	301379	520588	72.22%	8.609%
17	10.153	2823	2834	2858	rBV	130137	209463	29.06%	3.464%
18	10.326	2878	2888	2900	rVB3	11560	18524	2.57%	0.306%
19	11.185	3145	3155	3176	rBV	280953	456636	63.35%	7.552%
20	11.561	3258	3272	3293	rBV	285607	466758	64.75%	7.719%




Sum of corrected areas: 6046909

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035205.D
Acq On : 15 Apr 2024 18:30
Operator : SY/MD
Sample : P2057-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

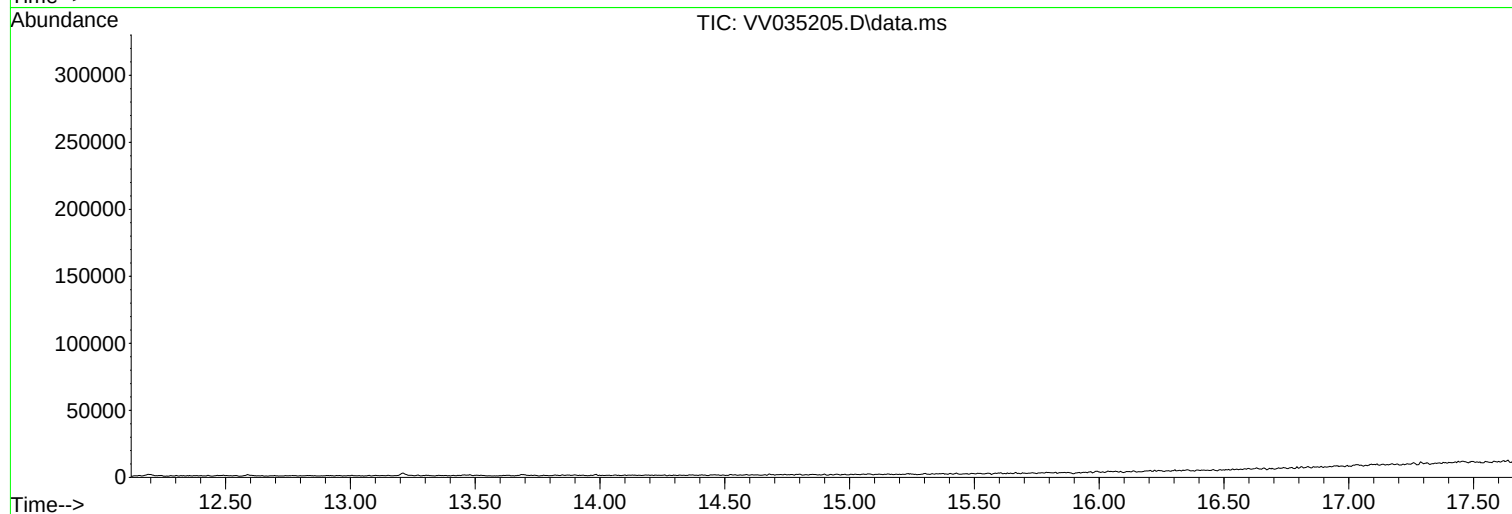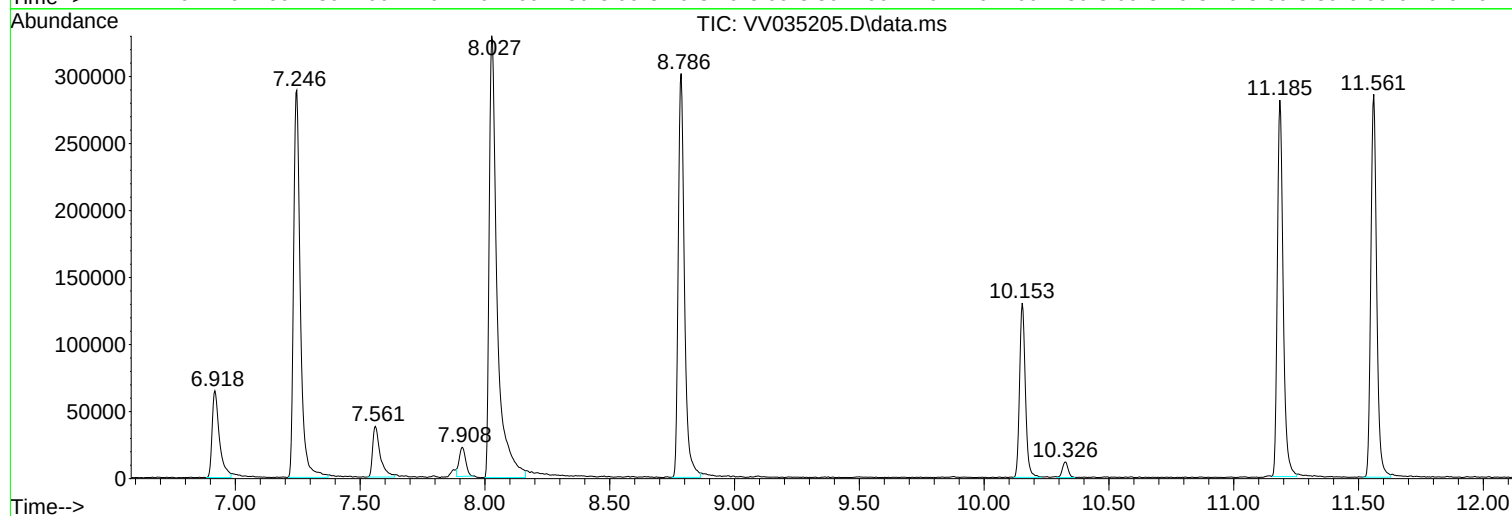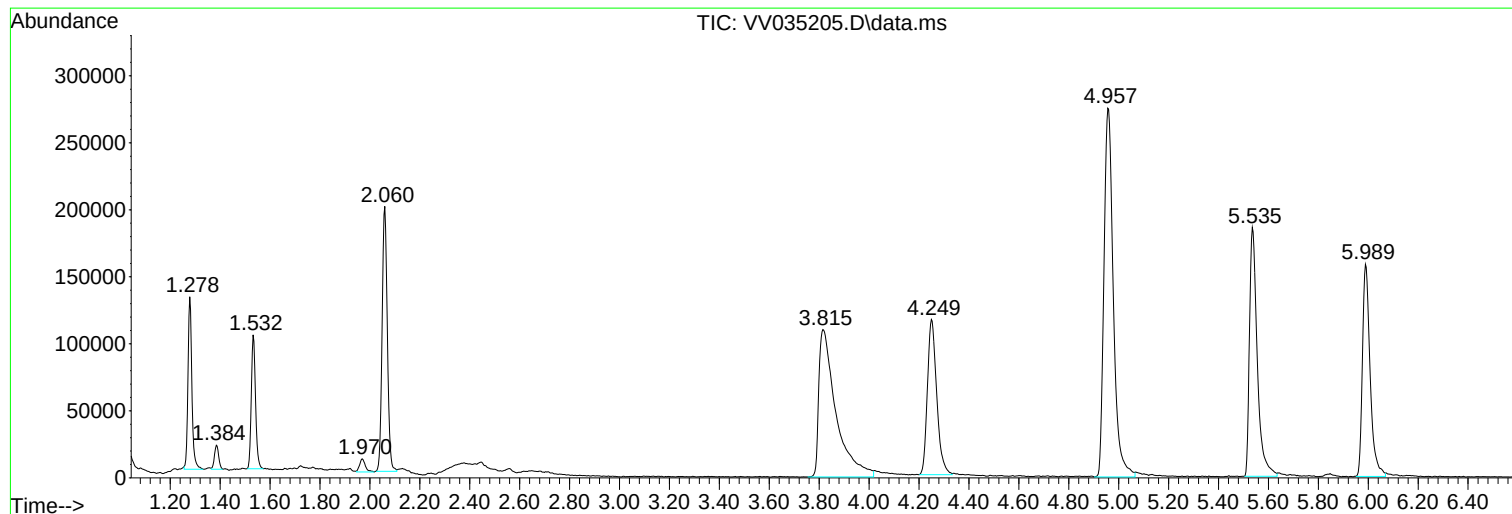

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035205.D
Acq On : 15 Apr 2024 18:30
Operator : SY/MD
Sample : P2057-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035205.D
Acq On : 15 Apr 2024 18:30
Operator : SY/MD
Sample : P2057-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc