

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
 Data File : VV035207.D
 Acq On : 15 Apr 2024 19:18
 Operator : SY/MD
 Sample : P2057-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV035207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	29	rVB5	7143	10633	1.36%	0.167%
2	1.278	67	74	88	rVB	144052	151435	19.35%	2.382%
3	1.384	102	107	114	rVB	10378	11319	1.45%	0.178%
4	1.532	146	153	167	rVB	112570	134401	17.17%	2.114%
5	1.970	282	289	299	rVB	18614	27023	3.45%	0.425%
6	2.060	306	317	334	rBV	219841	319619	40.83%	5.027%
7	3.818	847	864	913	rBV2	73355	360131	46.01%	5.665%
8	4.249	982	998	1022	rBV	127480	332217	42.44%	5.225%
9	4.957	1203	1218	1250	rBV2	302754	782766	100.00%	12.312%
10	5.535	1385	1398	1429	rBV	208533	452794	57.85%	7.122%
11	5.989	1526	1539	1562	rBV	174315	375336	47.95%	5.904%
12	6.918	1815	1828	1861	rBV	71312	149737	19.13%	2.355%
13	7.243	1919	1929	1967	rBV	332362	612603	78.26%	9.636%
14	7.558	2019	2027	2054	rBV2	40092	84167	10.75%	1.324%
15	7.915	2129	2138	2151	rVB5	7263	14136	1.81%	0.222%
16	8.027	2161	2173	2217	rBV	327845	719417	91.91%	11.316%
17	8.786	2398	2409	2435	rBV	336693	579797	74.07%	9.120%
18	10.153	2823	2834	2852	rBV	134759	214658	27.42%	3.376%
19	10.323	2876	2887	2900	rVB2	5533	9131	1.17%	0.144%
20	11.185	3145	3155	3179	rBV	314097	500055	63.88%	7.865%
21	11.561	3261	3272	3294	rBV	317164	516294	65.96%	8.121%




Sum of corrected areas: 6357669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035207.D
Acq On : 15 Apr 2024 19:18
Operator : SY/MD
Sample : P2057-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

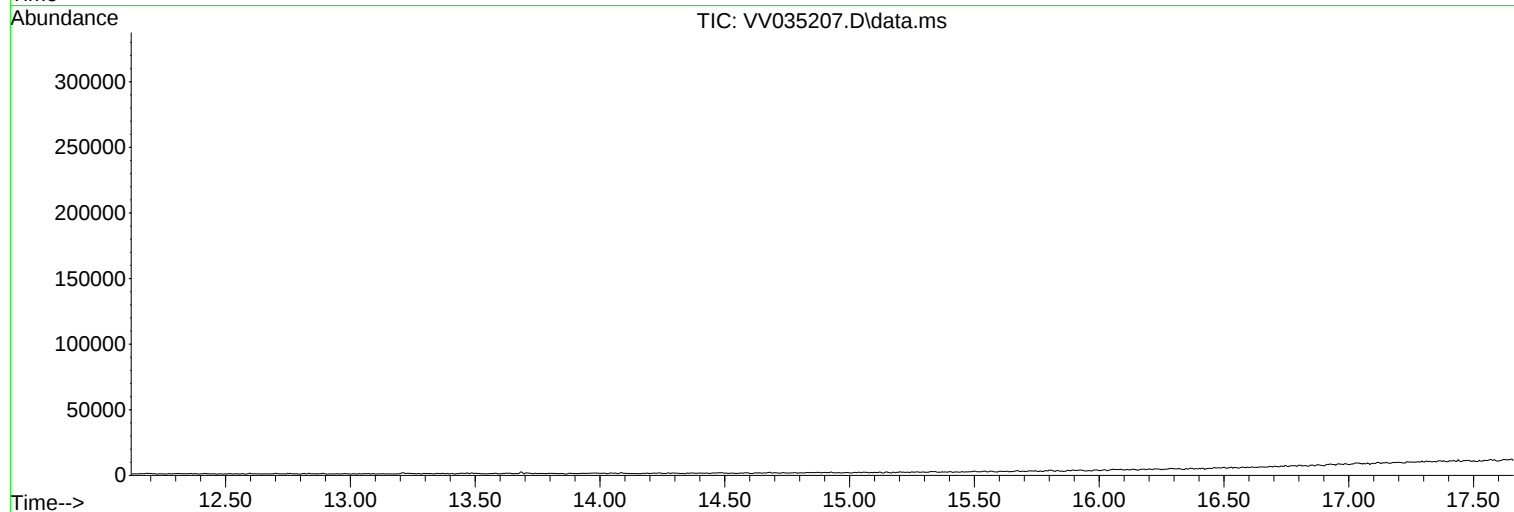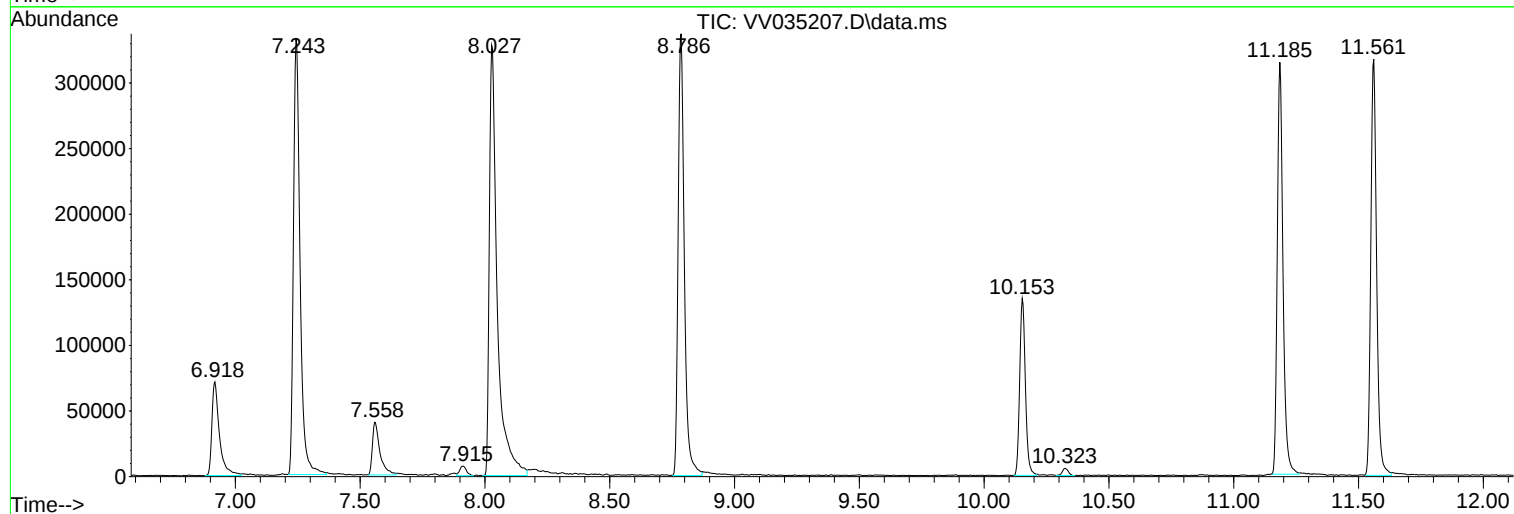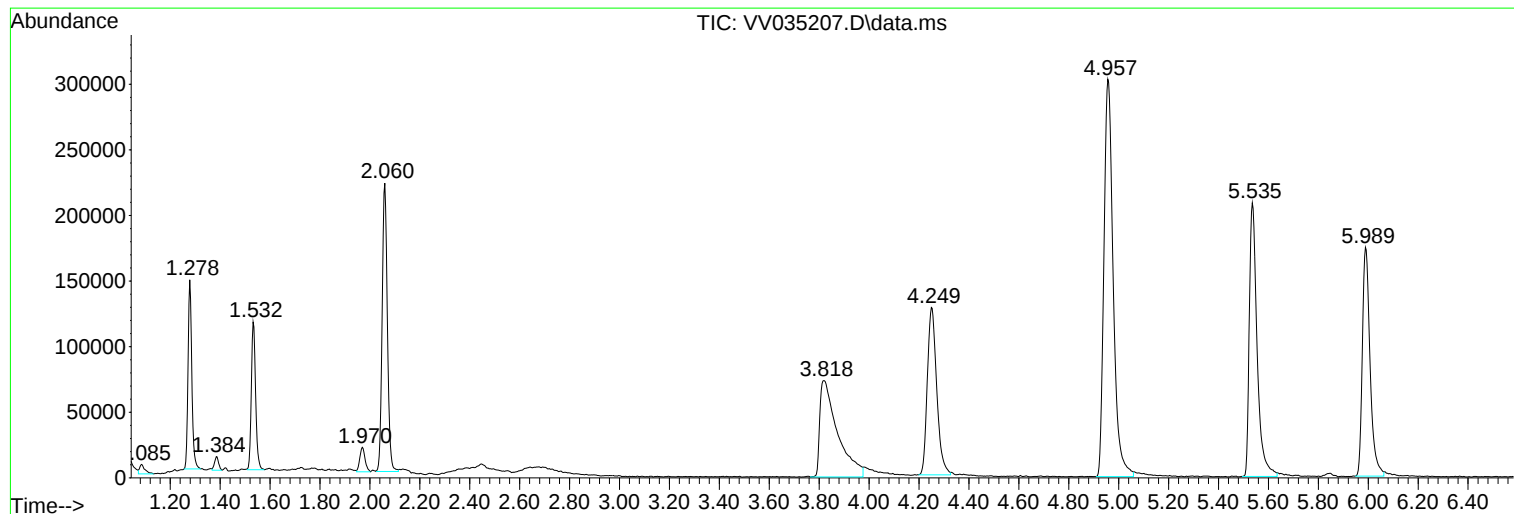

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035207.D
Acq On : 15 Apr 2024 19:18
Operator : SY/MD
Sample : P2057-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035207.D
Acq On : 15 Apr 2024 19:18
Operator : SY/MD
Sample : P2057-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
