

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
 Data File : VV035210.D
 Acq On : 15 Apr 2024 20:30
 Operator : SY/MD
 Sample : P2032-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOME7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV035210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	41	47	52	rBV	9177	9672	1.24%	0.154%
2	1.278	67	74	91	rVB	140025	149562	19.19%	2.375%
3	1.384	102	107	114	rBV	10858	12349	1.58%	0.196%
4	1.532	145	153	168	rVB	109288	128586	16.50%	2.042%
5	2.060	306	317	335	rBV	208501	303493	38.93%	4.820%
6	2.449	430	438	450	rVB2	5512	9564	1.23%	0.152%
7	3.815	848	863	918	rBV2	72143	332228	42.62%	5.276%
8	4.249	982	998	1029	rBV	129235	336124	43.12%	5.338%
9	4.513	1062	1080	1106	rBV2	46815	123832	15.89%	1.966%
10	4.957	1199	1218	1259	rBV2	299793	779510	100.00%	12.379%
11	5.535	1387	1398	1436	rBV	206266	452894	58.10%	7.192%
12	5.989	1527	1539	1563	rBV	176241	374684	48.07%	5.950%
13	6.918	1816	1828	1852	rBV	68226	143818	18.45%	2.284%
14	7.246	1918	1930	1958	rBV	317779	586232	75.21%	9.310%
15	7.561	2018	2028	2043	rBV	39898	78819	10.11%	1.252%
16	8.027	2164	2173	2209	rBV	329569	708225	90.86%	11.247%
17	8.786	2398	2409	2435	rBV	333319	570373	73.17%	9.058%
18	10.153	2822	2834	2852	rBV	133067	215216	27.61%	3.418%
19	11.185	3145	3155	3182	rBV	299242	486137	62.36%	7.720%
20	11.561	3257	3272	3292	rBV	305637	495761	63.60%	7.873%




Sum of corrected areas: 6297079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035210.D
Acq On : 15 Apr 2024 20:30
Operator : SY/MD
Sample : P2032-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0ME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

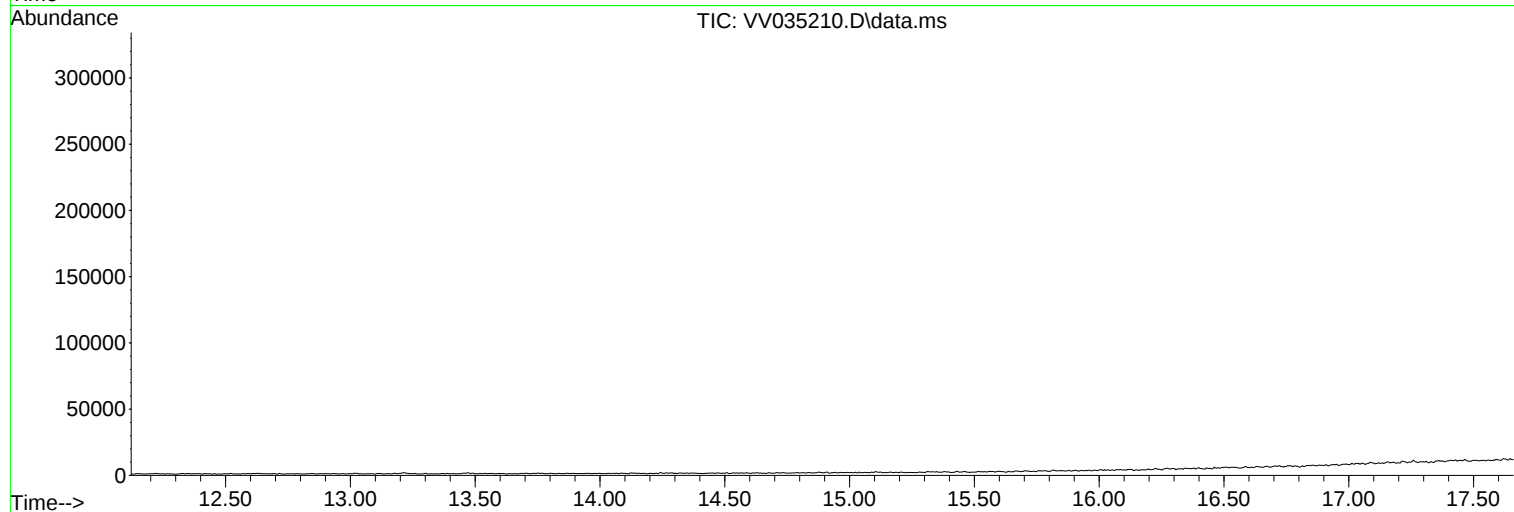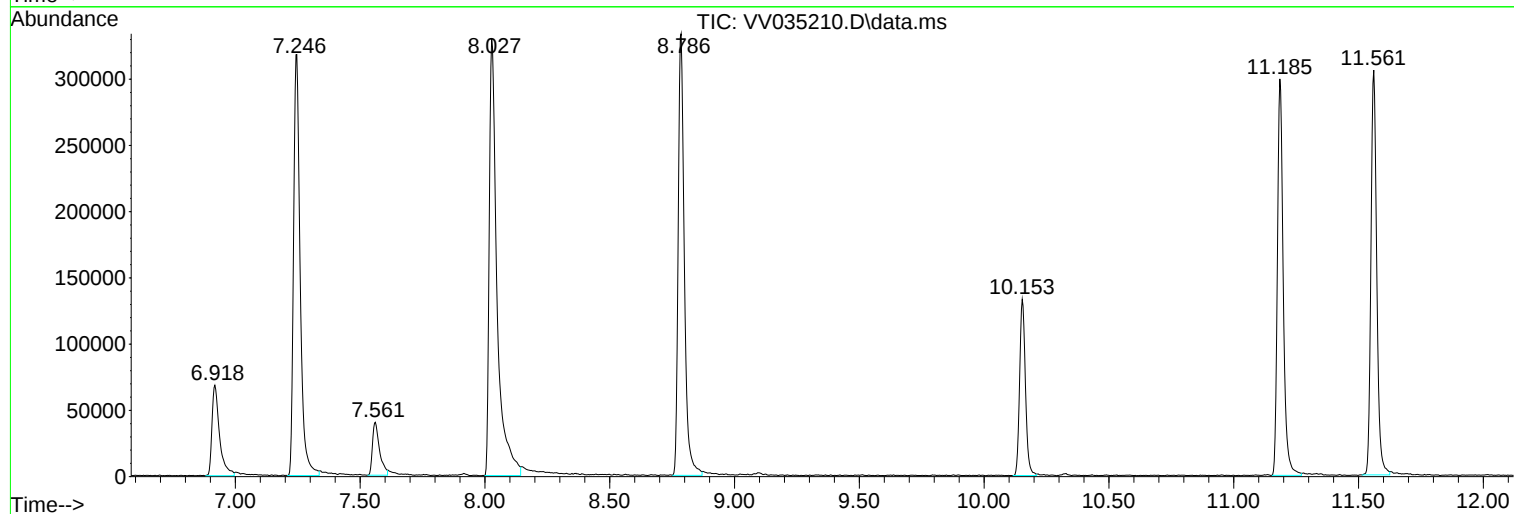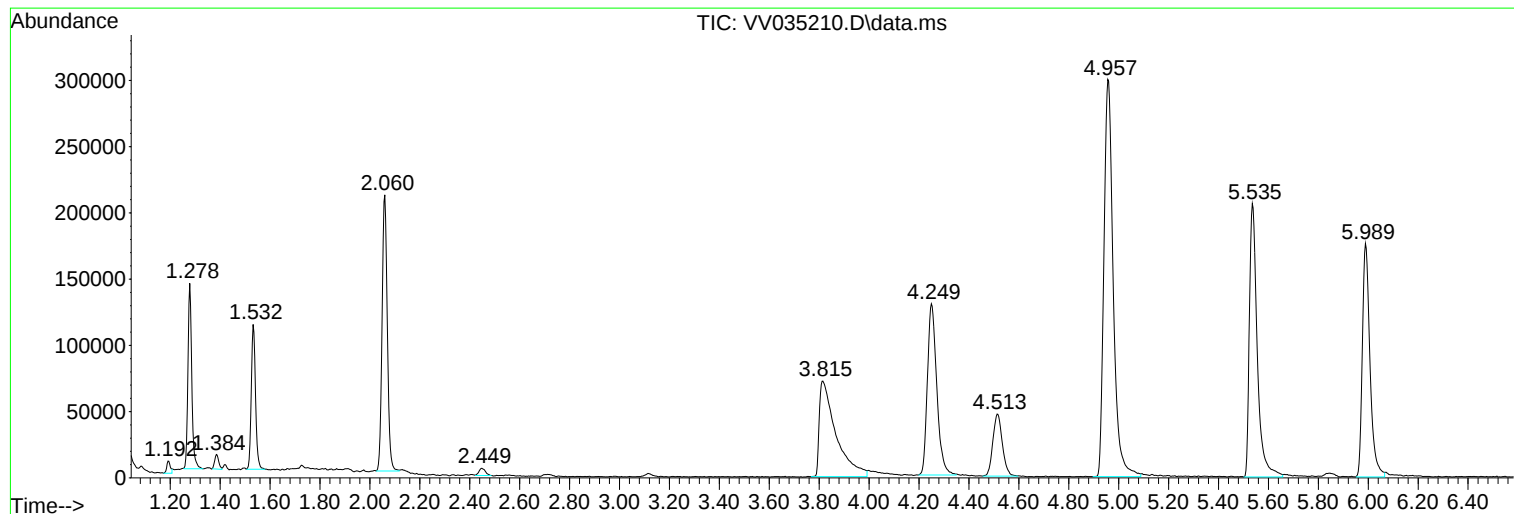

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035210.D
Acq On : 15 Apr 2024 20:30
Operator : SY/MD
Sample : P2032-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0ME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035210.D
Acq On : 15 Apr 2024 20:30
Operator : SY/MD
Sample : P2032-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0ME7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc