

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
 Data File : VV035211.D
 Acq On : 15 Apr 2024 20:54
 Operator : SY/MD
 Sample : P2032-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0ME8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rBV	136991	142996	18.57%	2.359%
2	1.384	103	107	114	rVB	10187	10019	1.30%	0.165%
3	1.532	146	153	170	rVB	110273	131035	17.02%	2.161%
4	2.060	306	317	336	rBV	210760	306180	39.76%	5.050%
5	2.449	429	438	451	rVB	5011	8788	1.14%	0.145%
6	3.825	852	866	895	rBV2	55901	255760	33.21%	4.219%
7	4.249	983	998	1025	rBV	123372	326643	42.42%	5.388%
8	4.957	1200	1218	1254	rBV2	298833	770066	100.00%	12.701%
9	5.535	1386	1398	1428	rBV	203288	442718	57.49%	7.302%
10	5.989	1526	1539	1573	rBV	170510	372132	48.32%	6.138%
11	6.918	1816	1828	1856	rBV	68001	143051	18.58%	2.359%
12	7.243	1917	1929	1951	rBV	311910	573813	74.51%	9.464%
13	7.561	2017	2028	2047	rBV	40226	82329	10.69%	1.358%
14	8.030	2164	2174	2221	rBV	318856	719822	93.48%	11.873%
15	8.786	2398	2409	2437	rBV	334745	564879	73.35%	9.317%
16	10.152	2823	2834	2848	rBV	132429	212602	27.61%	3.507%
17	11.185	3145	3155	3184	rBV	299155	488836	63.48%	8.063%
18	11.503	3241	3254	3261	rBV5	5908	12346	1.60%	0.204%
19	11.561	3261	3272	3296	rVB	309056	498783	64.77%	8.227%




Sum of corrected areas: 6062798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035211.D
Acq On : 15 Apr 2024 20:54
Operator : SY/MD
Sample : P2032-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0ME8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

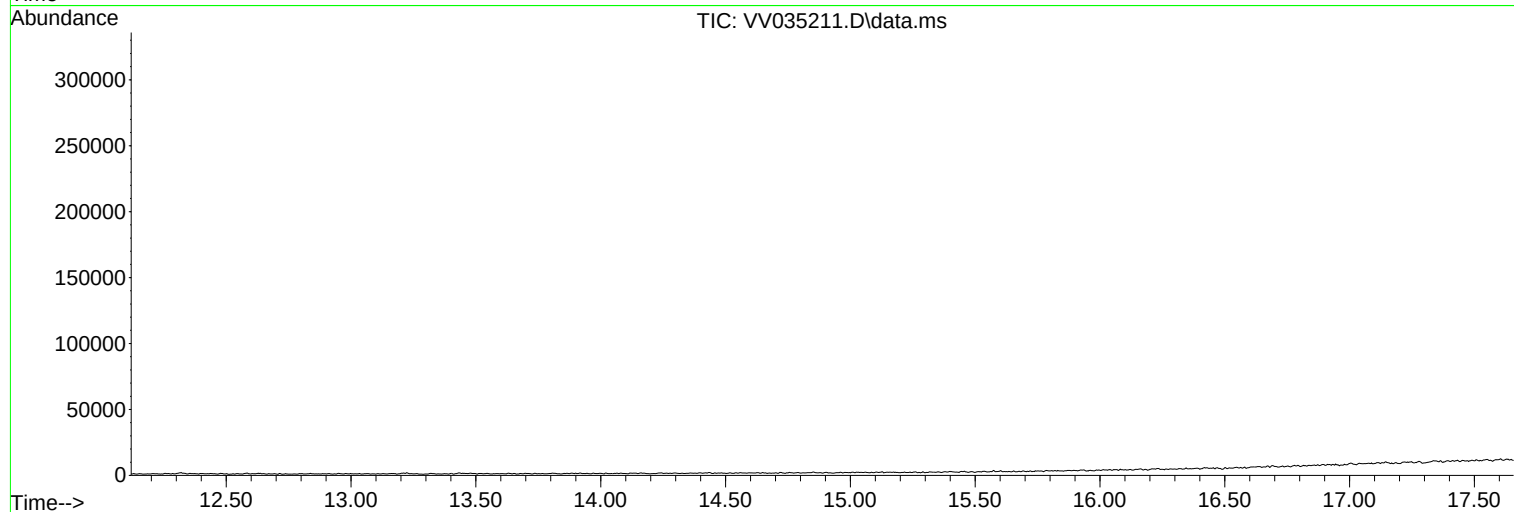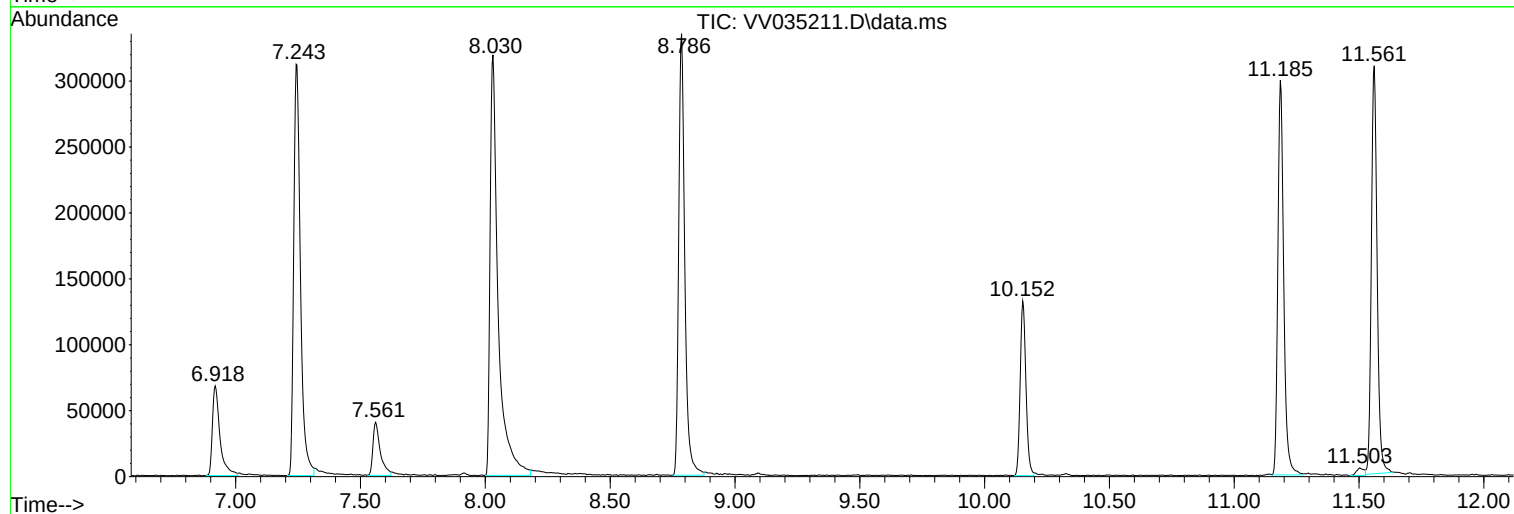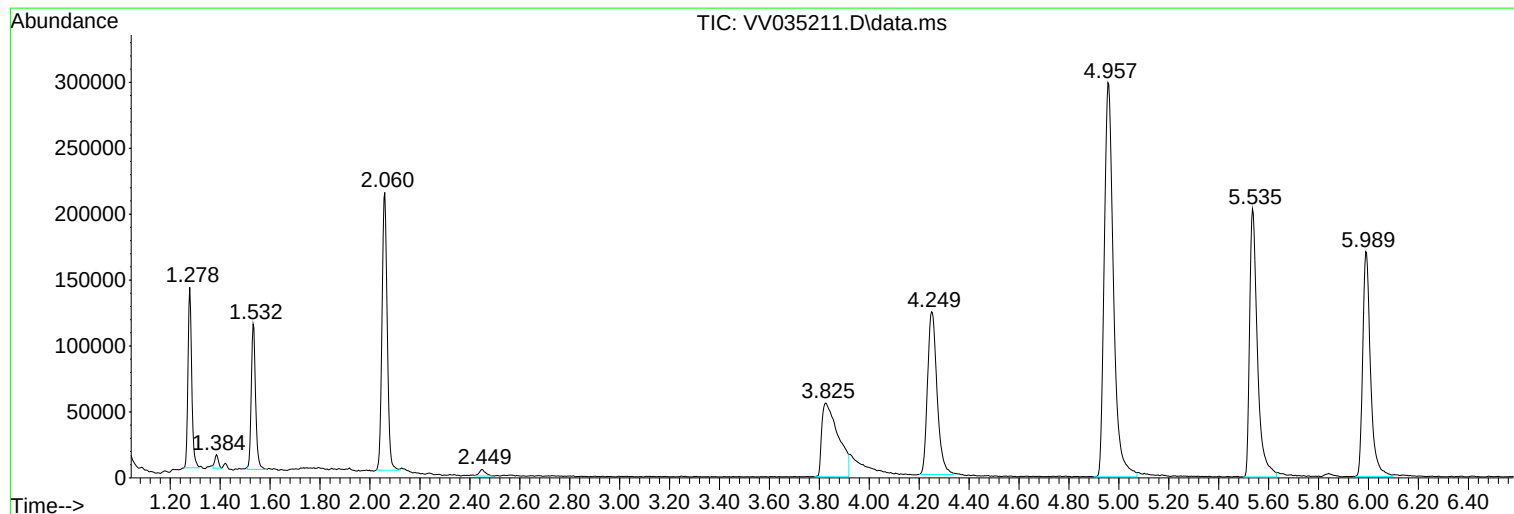

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035211.D
Acq On : 15 Apr 2024 20:54
Operator : SY/MD
Sample : P2032-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0ME8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035211.D
Acq On : 15 Apr 2024 20:54
Operator : SY/MD
Sample : P2032-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0ME8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc