

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
 Data File : VV035223.D
 Acq On : 16 Apr 2024 01:42
 Operator : SY/MD
 Sample : VIBLK333
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK333

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	42	54	62	rBV2	5467	10815	1.45%	0.182%
2	1.278	67	74	90	rVV	133192	144492	19.36%	2.427%
3	1.536	146	154	170	rBV	103948	125989	16.88%	2.116%
4	2.060	307	317	333	rVB	208443	303687	40.70%	5.101%
5	2.449	428	438	453	rVB	16297	28822	3.86%	0.484%
6	3.818	855	864	906	rBV	53528	250064	33.51%	4.201%
7	4.249	982	998	1025	rBV	122206	326746	43.79%	5.489%
8	4.957	1204	1218	1257	rBV2	286209	746205	100.00%	12.535%
9	5.535	1387	1398	1431	rBV	204459	443385	59.42%	7.448%
10	5.989	1526	1539	1565	rBV	167548	364001	48.78%	6.115%
11	6.918	1818	1828	1850	rBV	65105	132596	17.77%	2.227%
12	7.243	1918	1929	1960	rBV	310161	572946	76.78%	9.624%
13	7.558	2017	2027	2053	rBV	37601	79588	10.67%	1.337%
14	8.027	2164	2173	2221	rBV	293226	666436	89.31%	11.195%
15	8.786	2396	2409	2429	rBV	332832	567027	75.99%	9.525%
16	10.153	2823	2834	2858	rBV	125136	207047	27.75%	3.478%
17	10.323	2878	2887	2899	rBV3	5123	7779	1.04%	0.131%
18	11.185	3143	3155	3182	rBV	304876	492137	65.95%	8.267%
19	11.561	3260	3272	3294	rBV	296484	483301	64.77%	8.119%




Sum of corrected areas: 5953063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035223.D
Acq On : 16 Apr 2024 01:42
Operator : SY/MD
Sample : VIBLK333
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

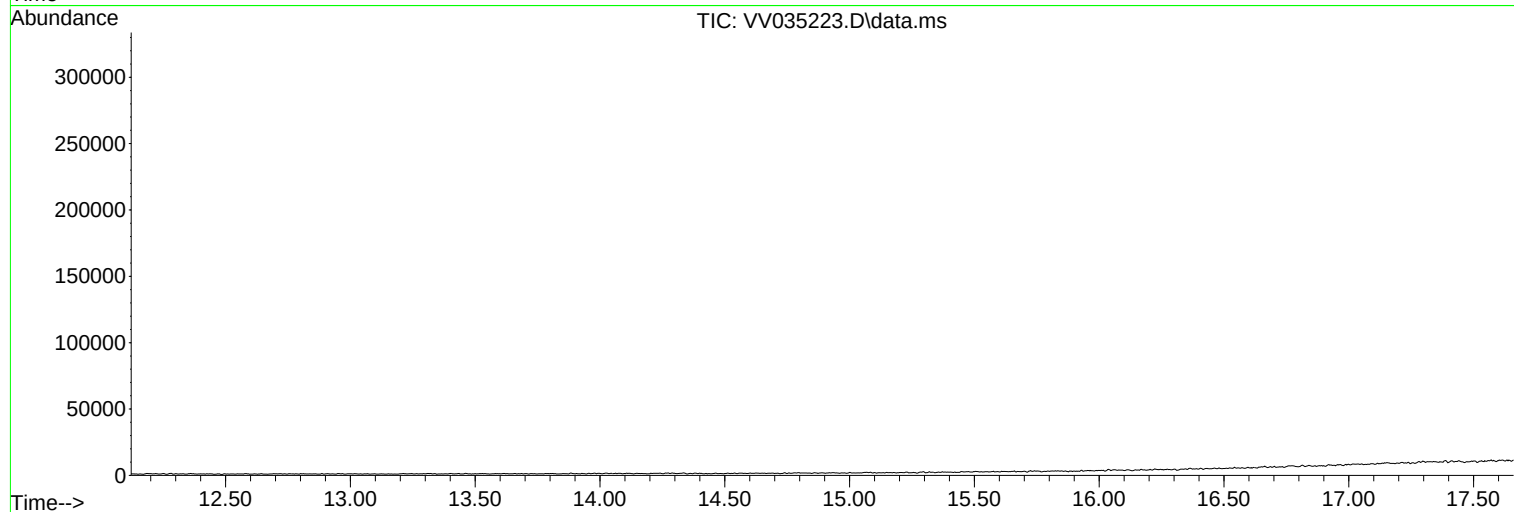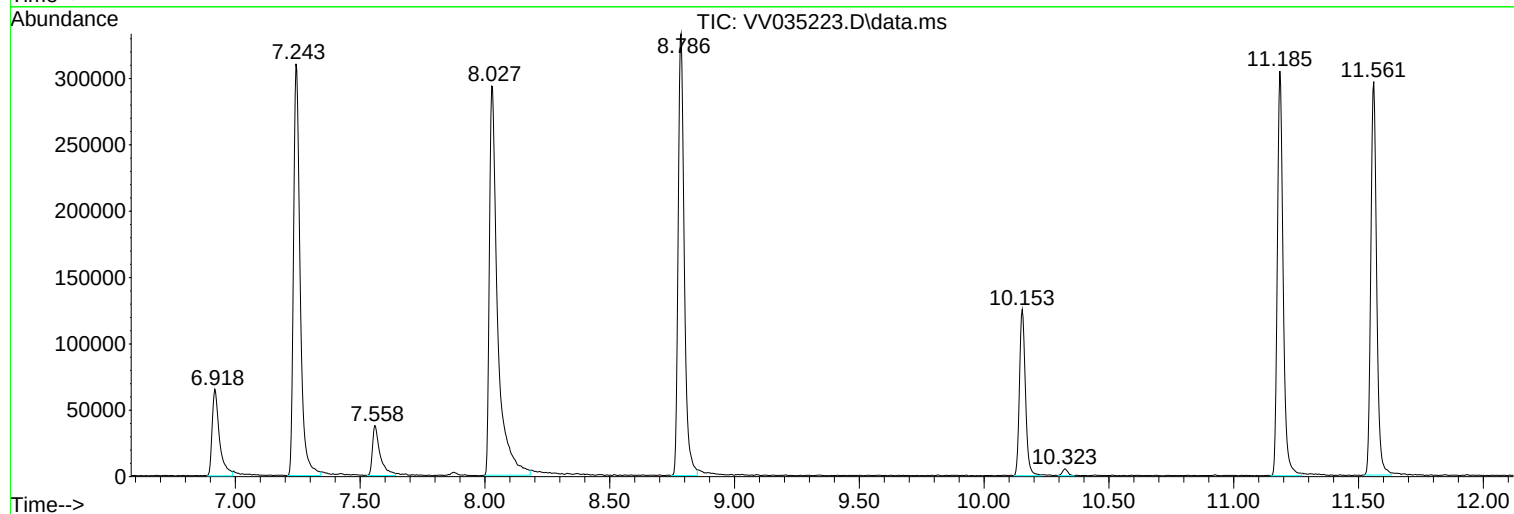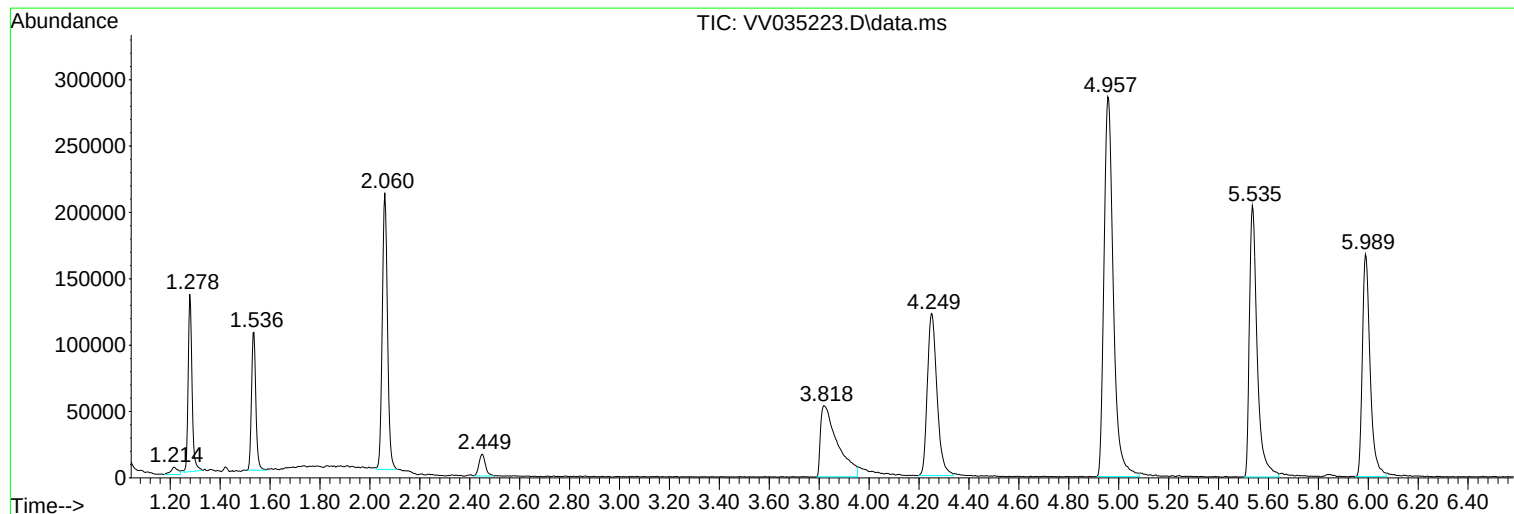

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035223.D
Acq On : 16 Apr 2024 01:42
Operator : SY/MD
Sample : VIBLK333
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035223.D
Acq On : 16 Apr 2024 01:42
Operator : SY/MD
Sample : VIBLK333
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
