
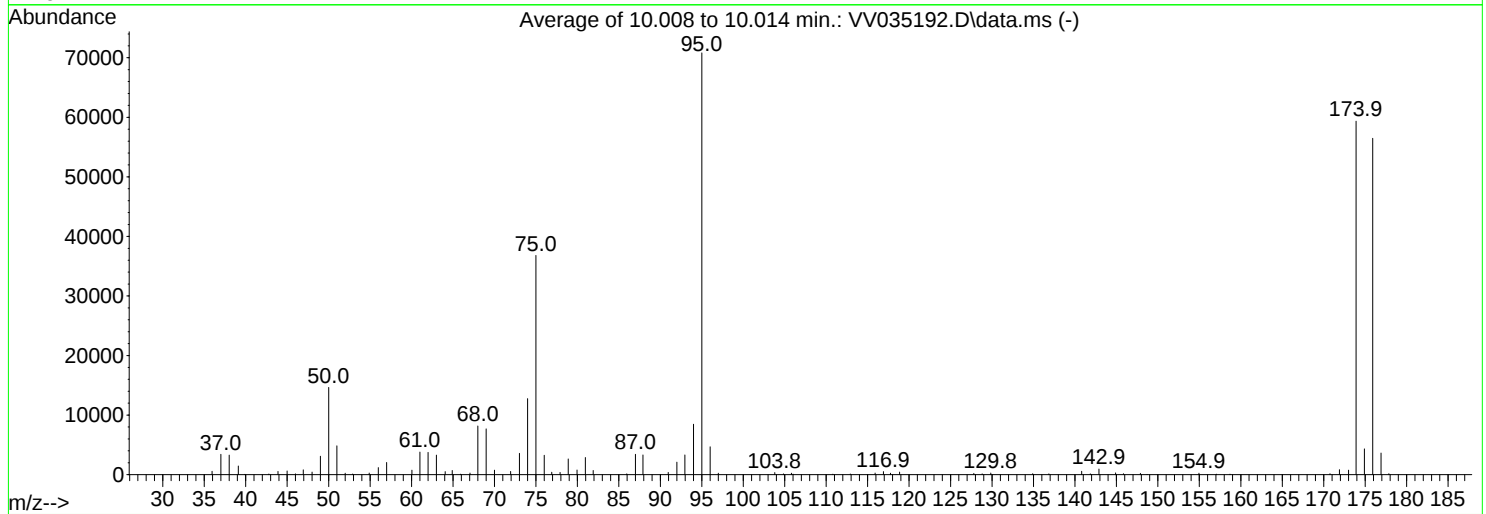


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041524\
Data File : VV035192.D
Acq On : 15 Apr 2024 10:59
Operator : SY/MD
Sample : BFB268
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB268

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR041524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 17 02:28:28 2024

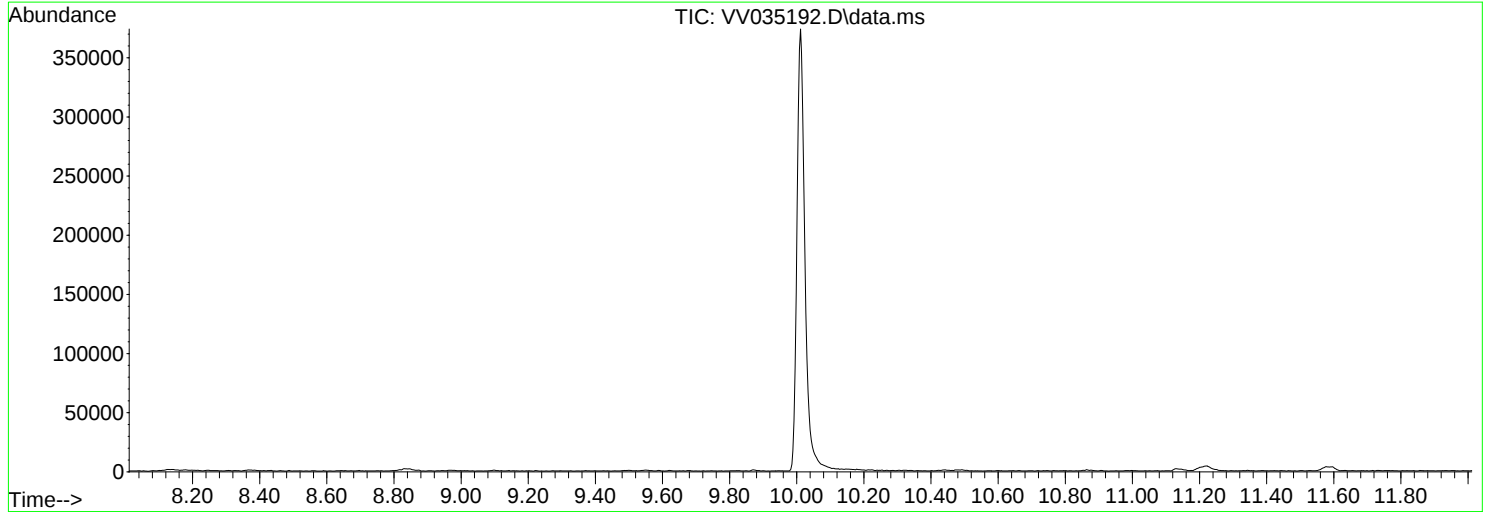

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	14643	PASS
75	95	30	80	52.0	36800	PASS
95	95	100	100	100.0	70824	PASS
96	95	5	9	6.6	4681	PASS
173	174	0.00	2	1.3	754	PASS
174	95	50	120	83.8	59360	PASS
175	174	5	9	7.3	4334	PASS
176	174	95	105	95.1	56480	PASS
177	176	5	10	6.5	3643	PASS

m/z	Abundance
39.90	297.0
43.90	467.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
36.00	592.0
37.00	3340.0
38.00	3324.0
39.10	1524.0
39.90	352.0
42.80	128.0
43.90	974.0
45.00	611.0
46.00	141.0
47.00	833.0
48.00	415.0
49.00	3238.0
50.00	14738.0
51.00	4991.0
52.00	268.0
52.90	115.0
54.90	252.0
56.00	1090.0
57.00	2095.0
60.00	753.0
61.00	3701.0
62.00	3854.0
63.00	3312.0
64.10	521.0
64.90	689.0
67.00	263.0
68.00	8046.0
69.00	7826.0
70.00	750.0
71.90	570.0
73.00	3660.0
74.00	12705.0
75.00	36936.0
76.00	3349.0
76.90	380.0
77.90	376.0
78.90	2480.0
80.00	768.0
81.00	2920.0
81.90	653.0
86.00	123.0
87.00	3651.0
87.90	3373.0
90.90	389.0
92.00	2144.0
93.00	3267.0
94.00	8496.0
95.00	69568.0
96.00	4627.0
97.00	222.0
103.80	373.0
104.90	124.0
105.80	361.0
112.90	104.0
115.90	286.0
116.90	491.0
117.80	221.0
118.80	439.0
127.80	199.0
128.80	166.0
129.90	228.0
134.80	163.0
136.90	161.0
140.80	588.0
141.80	130.0
142.90	963.0
144.90	324.0
145.80	155.0
147.90	213.0
148.70	100.0
154.90	240.0
157.10	133.0
158.70	139.0
170.70	140.0
171.90	803.0
173.00	681.0
173.90	57208.0
174.90	4338.0
175.90	54448.0
176.90	3519.0
177.90	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
35.90	552.0
37.00	3501.0
38.00	3384.0
39.10	1486.0
39.90	363.0
42.80	128.0
44.00	1001.0
45.00	625.0
46.00	132.0
46.90	845.0
48.00	446.0
49.00	3181.0
50.00	15165.0
51.00	5028.0
52.00	249.0
52.90	140.0
54.90	283.0
56.00	1223.0
57.00	2102.0
60.10	810.0
61.00	3963.0
62.00	3903.0
63.00	3440.0
64.10	517.0
64.90	703.0
65.90	108.0
67.00	283.0
68.00	8396.0
69.00	7942.0
70.00	761.0
72.00	552.0
73.00	3715.0
74.00	13308.0
75.00	38024.0
76.00	3395.0
76.90	412.0
77.90	389.0
78.90	2741.0
80.00	795.0
81.00	2995.0
81.90	726.0
86.00	141.0
87.00	3556.0
87.90	3456.0
90.90	384.0
92.00	2142.0
92.90	3379.0
94.00	8706.0
95.00	73096.0
96.00	4892.0
97.00	247.0
103.80	354.0
104.80	140.0
105.80	335.0
110.80	117.0
112.90	130.0
115.90	293.0
116.90	511.0
117.70	249.0
118.90	466.0
127.80	218.0
128.80	145.0
129.80	264.0
134.90	159.0
136.90	137.0
140.80	570.0
141.90	145.0
142.90	1003.0
144.90	311.0
145.90	187.0
147.90	240.0
155.00	245.0
157.00	116.0
158.70	125.0
170.80	176.0
171.90	859.0
173.00	792.0
173.90	61584.0
174.90	4436.0
175.90	58360.0
176.90	3749.0
177.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
35.90	538.0
37.00	3375.0
38.00	3138.0
39.10	1351.0
39.90	367.0
42.80	106.0
44.00	1038.0
45.00	643.0
46.00	105.0
46.90	728.0
48.00	461.0
49.00	2871.0
50.00	14025.0
51.00	4507.0
52.00	219.0
52.90	115.0
54.90	254.0
56.00	1221.0
57.00	1923.0
60.00	678.0
61.00	3734.0
62.00	3494.0
63.00	3076.0
64.00	529.0
64.90	714.0
65.90	119.0
67.10	252.0
68.00	8070.0
69.00	7312.0
70.00	718.0
72.00	486.0
73.00	3372.0
74.00	12280.0
75.00	35440.0
76.00	3047.0
76.90	416.0
77.90	329.0
78.90	2705.0
79.90	777.0
80.90	2700.0
81.90	691.0
85.90	133.0
87.00	3028.0
87.90	3067.0
91.00	322.0
92.00	1970.0
92.90	3296.0
94.00	8195.0
95.00	69808.0
96.00	4525.0
97.00	234.0
103.80	309.0
104.80	126.0
106.00	278.0
110.80	114.0
112.90	115.0
115.90	229.0
116.90	517.0
117.70	257.0
118.90	425.0
127.80	219.0
128.80	119.0
129.80	300.0
135.00	164.0
136.80	109.0
140.80	520.0
141.80	135.0
142.90	872.0
144.90	284.0
145.90	180.0
147.90	230.0
155.00	216.0
170.80	183.0
171.90	853.0
173.00	790.0
173.90	59288.0
174.90	4228.0
175.90	56632.0
176.90	3661.0
177.80	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268