

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041723\
 Data File : VW030597.D
 Acq On : 17 Apr 2023 18:36
 Operator : SY/MD
 Sample : 02360-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 18 02:51:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 18 02:45:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	246090	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	235981	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	105463	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	83930	46.524	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	93.040%		
7) Chloroethane-d5	1.539	69	70392	46.563	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.120%		
11) 1,1-Dichloroethene-d2	2.063	65	39261	45.891	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.780%		
21) 2-Butanone-d5	3.805	46	97143	98.037	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.040%		
24) Chloroform-d	4.259	84	150140	45.924	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.840%		
26) 1,2-Dichloroethane-d4	4.953	65	101570	48.323	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.640%		
32) Benzene-d6	4.969	84	281082	50.380	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.760%		
36) 1,2-Dichloropropane-d6	5.998	67	89094	51.408	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.820%		
41) Toluene-d8	7.252	98	243541	46.492	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.980%		
43) trans-1,3-Dichloroprop...	7.561	79	40652	46.539	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.080%		
47) 2-Hexanone-d5	8.034	63	60847	89.124	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.120%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	115445	45.907	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.820%		
66) 1,2-Dichlorobenzene-d4	11.570	152	90343	53.894	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	107.780%		
Target Compounds						Qvalue
3) Chloromethane	1.220	50	13095	4.718	ug/L	97
6) Bromomethane	1.497	94	2880	3.246	ug/L	95
9) Trichlorofluoromethane	2.072	101	4671	1.288	ug/L	84
10) 1,1,2-Trichloro-1,2,2-...	2.072	101	4783	2.510	ug/L #	86
12) 1,1-Dichloroethene	2.076	96	4349	2.524	ug/L #	1
20) cis-1,2-Dichloroethene	3.825	96	17503	9.250	ug/L	93
30) 1,1,1-Trichloroethane	4.522	97	279523	84.298	ug/L	99
31) Carbon tetrachloride	4.522	117	34687	11.700	ug/L	99
34) Trichloroethene	5.841	95	334388	179.398	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041723\
Data File : VV030597.D
Acq On : 17 Apr 2023 18:36
Operator : SY/MD
Sample : 02360-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 18 02:51:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 18 02:45:56 2023
Response via : Initial Calibration

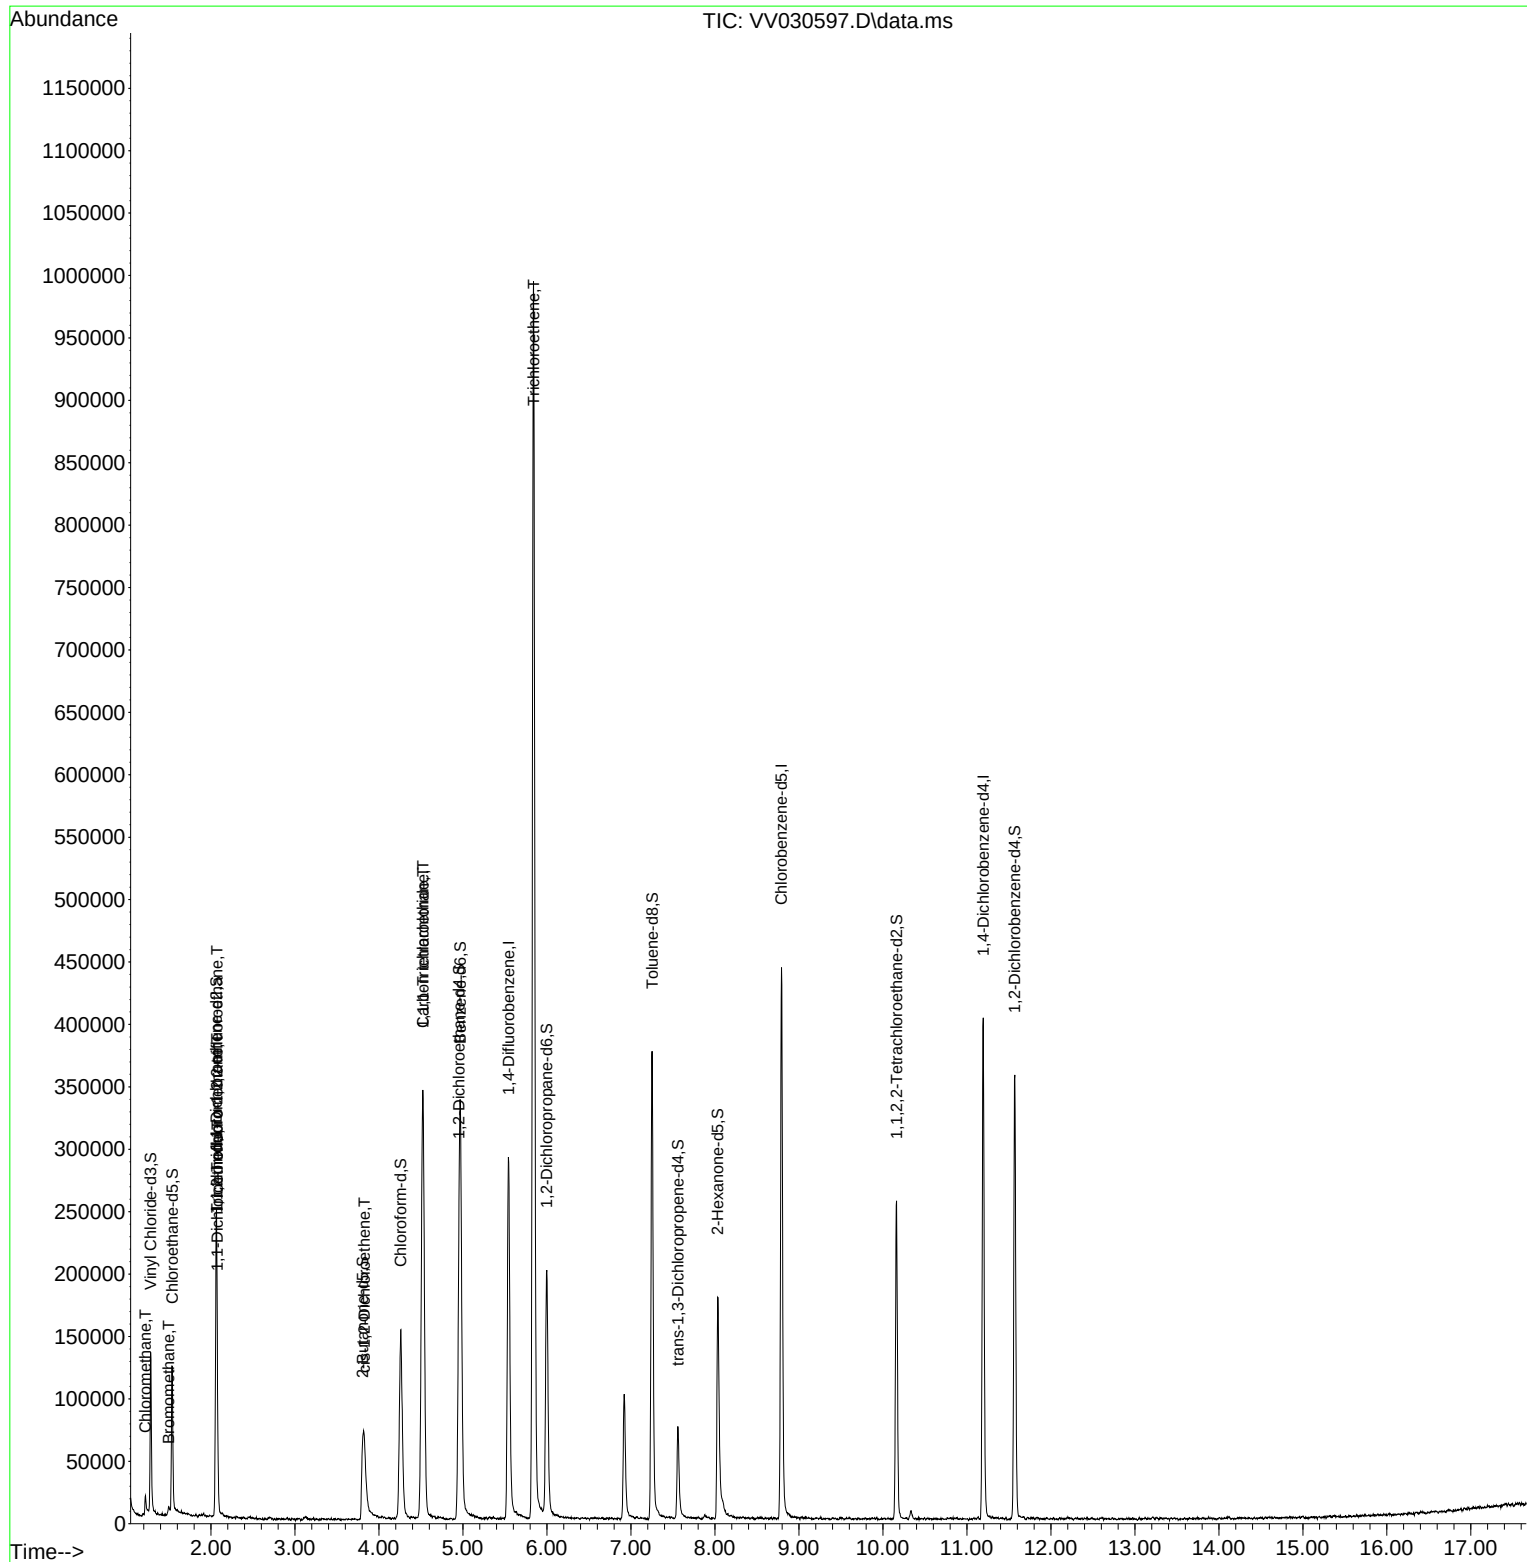

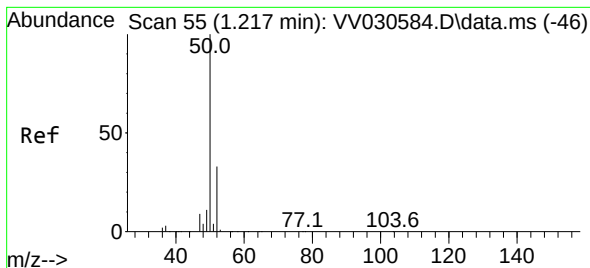

#3

Chloromethane

Concen: 4.718 ug/L

RT: 1.220 min Scan# 50

Delta R.T. 0.003 min

Lab File: VV030597.D

Acq: 17 Apr 2023 18:36

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 50 Resp: 13095

Ion Ratio Lower Upper

50 100

52 33.7 22.5 41.9

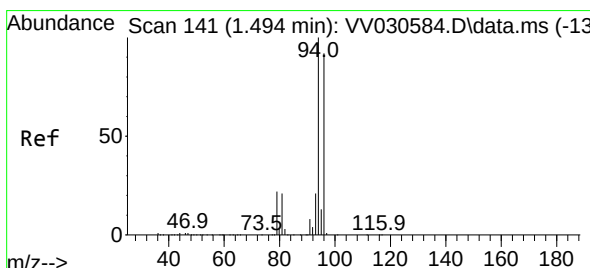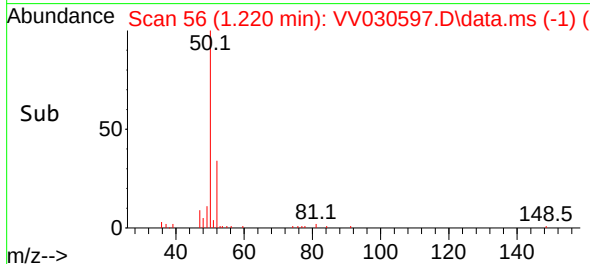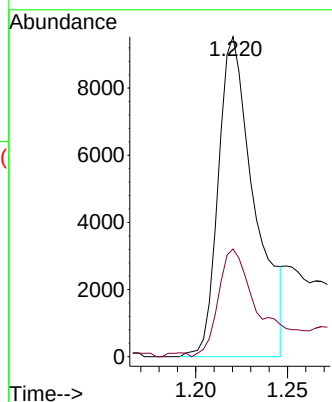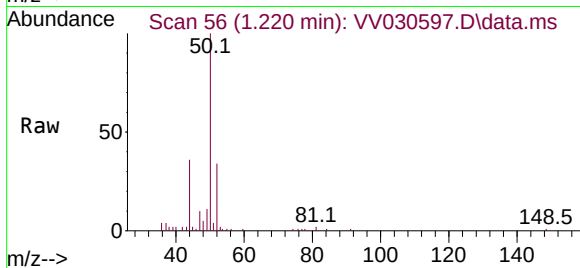

#6

Bromomethane

Concen: 3.246 ug/L

RT: 1.497 min Scan# 142

Delta R.T. 0.003 min

Lab File: VV030597.D




Acq: 17 Apr 2023 18:36


Tgt Ion: 94 Resp: 2880

Ion Ratio Lower Upper

94 100

96 89.8 66.3 123.1


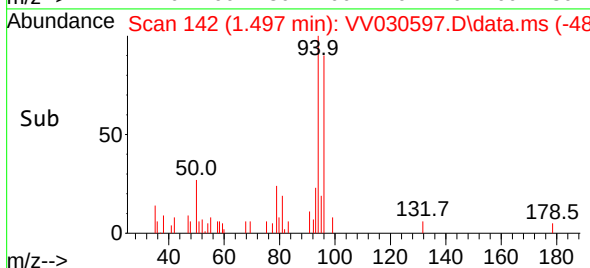
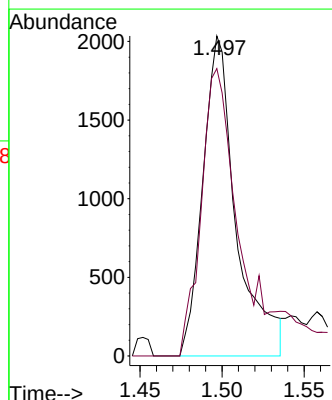
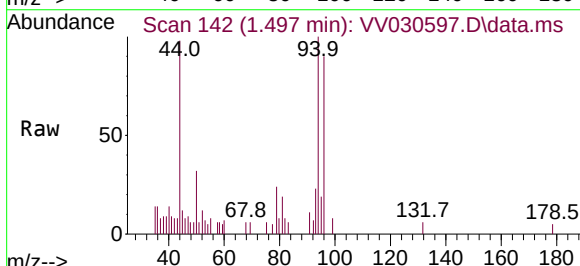


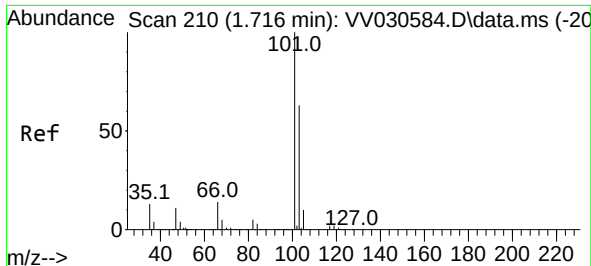

#9
 Trichlorofluoromethane
 Concen: 1.288 ug/L
 RT: 2.072 min Scan# 31
 Delta R.T. 0.357 min
 Lab File: VV030597.D
 Acq: 17 Apr 2023 18:36




Instrument :
 MSVOA_V
 ClientSampleId :


Tgt Ion:101 Resp: 4671
 Ion Ratio Lower Upper
 101 100
 103 51.6 51.4 77.0

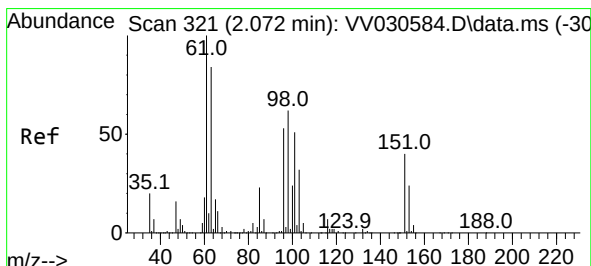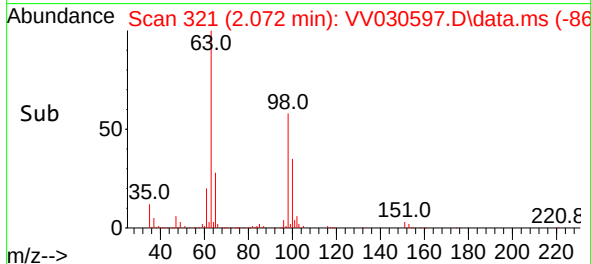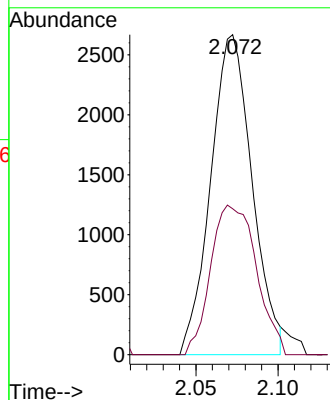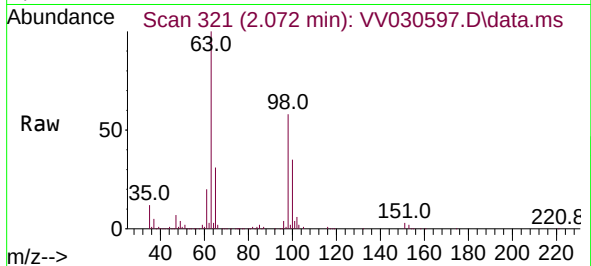

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 2.510 ug/L
 RT: 2.072 min Scan# 321
 Delta R.T. -0.000 min
 Lab File: VV030597.D
 Acq: 17 Apr 2023 18:36


Tgt Ion:101 Resp: 4783
 Ion Ratio Lower Upper
 101 100
 85 41.8 37.5 56.3
 151 63.3 63.5 95.3#

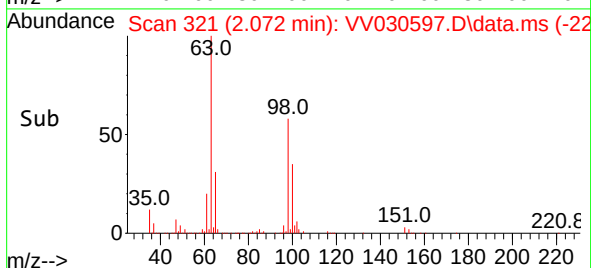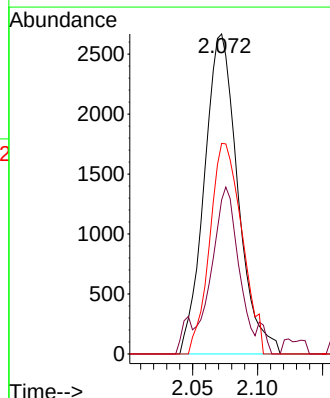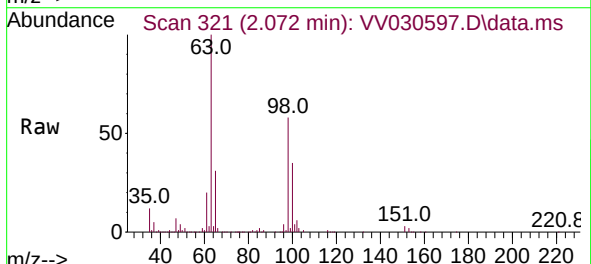



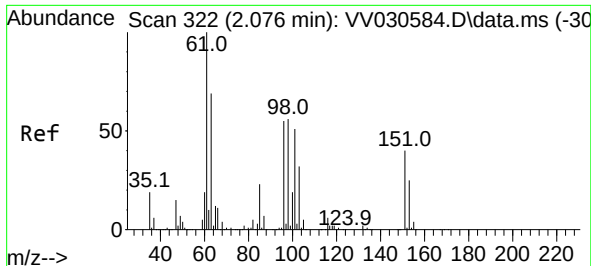


#12
1,1-Dichloroethene
Concen: 2.524 ug/L
RT: 2.076 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV030597.D
Acq: 17 Apr 2023 18:36

Instrument :
MSVOA_V
ClientSampleId :



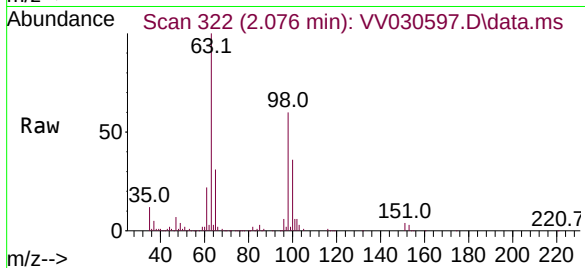



Tgt Ion: 96 Resp: 4349
Ion Ratio Lower Upper
96 100
61 352.0 131.9 245.0#
63 1628.8 99.8 185.3#

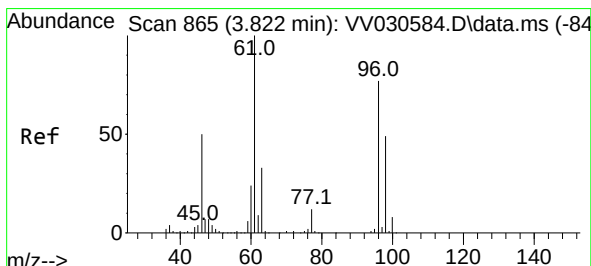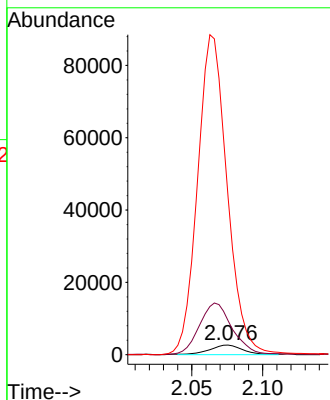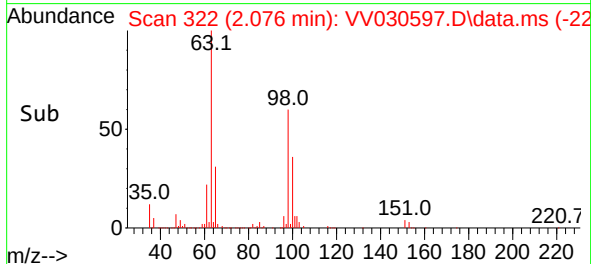

#20
cis-1,2-Dichloroethene
Concen: 9.250 ug/L
RT: 3.825 min Scan# 866
Delta R.T. 0.003 min
Lab File: VV030597.D
Acq: 17 Apr 2023 18:36

Tgt Ion: 96 Resp: 17503
Ion Ratio Lower Upper
96 100
61 124.7 92.3 171.3
98 59.1 45.9 85.3


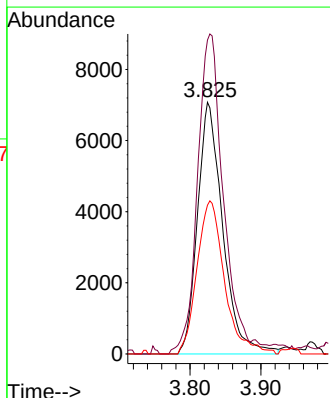
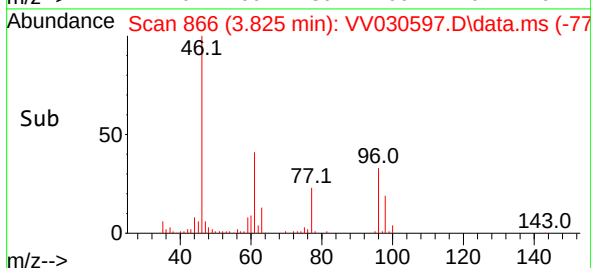
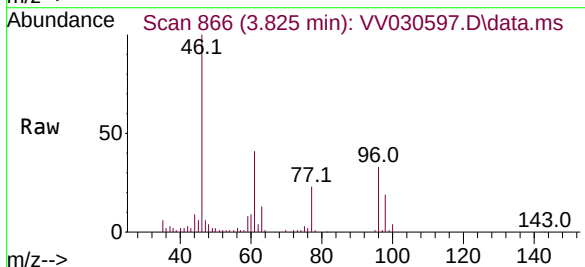


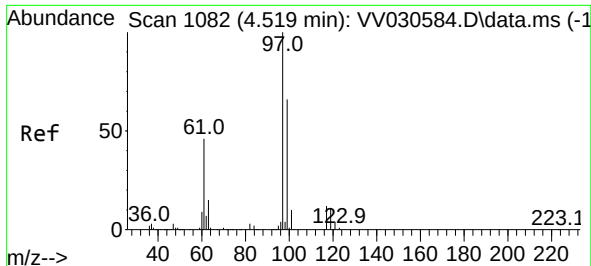

#30
1,1,1-Trichloroethane
Concen: 84.298 ug/L
RT: 4.522 min Scan# 1083
Delta R.T. 0.003 min
Lab File: VV030597.D
Acq: 17 Apr 2023 18:36




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 97 Resp: 279523
Ion Ratio Lower Upper
97 100
99 65.1 51.4 77.0
61 46.3 37.0 55.6

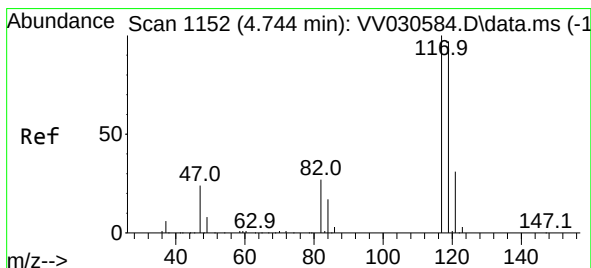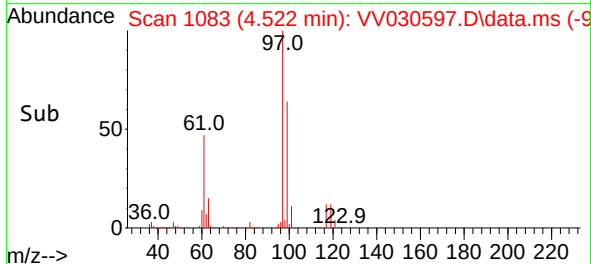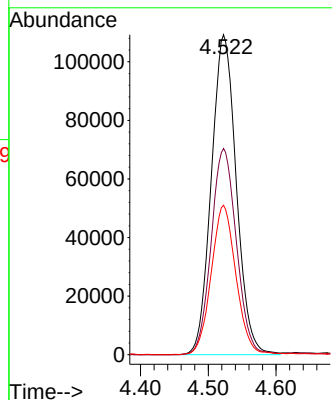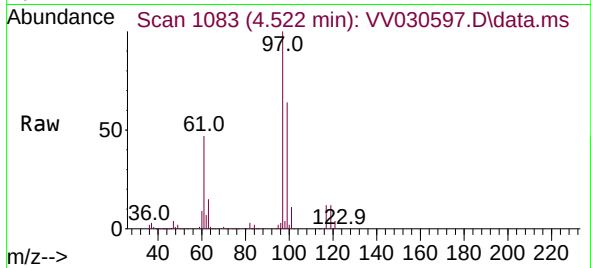

#31
Carbon tetrachloride
Concen: 11.700 ug/L
RT: 4.522 min Scan# 1083
Delta R.T. -0.222 min
Lab File: VV030597.D
Acq: 17 Apr 2023 18:36


Tgt Ion: 117 Resp: 34687
Ion Ratio Lower Upper
117 100
119 95.5 75.9 113.9

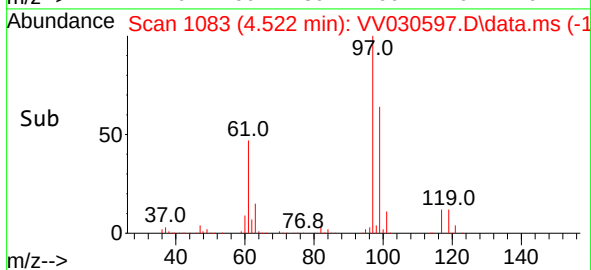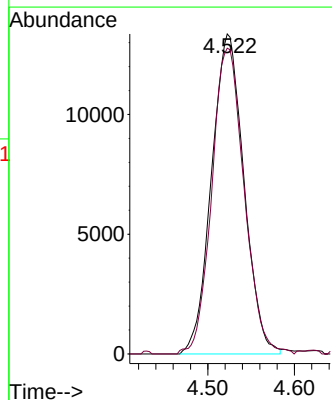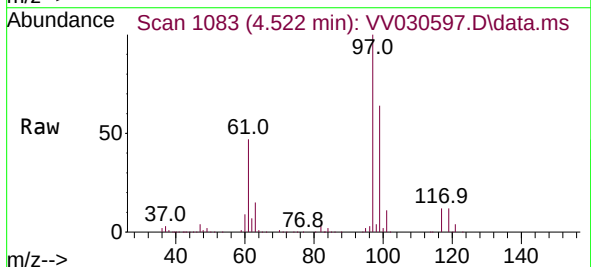

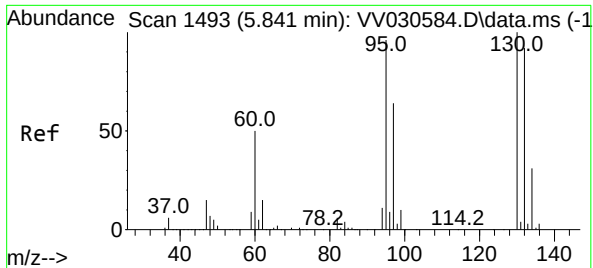

#34
 Trichloroethene
 Concen: 179.398 ug/L
 RT: 5.841 min Scan# 1493
 Delta R.T. -0.000 min
 Lab File: VV030597.D
 Acq: 17 Apr 2023 18:36

Instrument :
 MSVOA_V
 ClientSampleId :

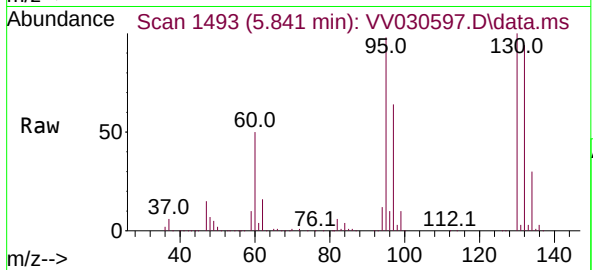

Tgt Ion: 95 Resp: 334388

Ion	Ratio	Lower	Upper
95	100		
97	64.9	45.8	85.2
132	95.8	70.6	131.2
130	102.2	70.9	131.7

